

# GDSN for the FDA Global Unique Device Identifier Database (GUDID)

## Implementation Guide

Version 1.1, May 2014  
Draft pending IP Review and Ratification







© GS1 AISBL

All rights reserved.

GS1 Global Office

Avenue Louise 326, bte 10

B-1050 Brussels, Belgium

## Disclaimer

GS1, under its IP Policy, seeks to avoid uncertainty regarding intellectual property claims by requiring the participants in the Work Group that developed this **GDSN for the FDA Global Unique Device Identifier Database (GUDID)** to agree to grant to GS1 members a royalty-free license or a RAND license to Necessary Claims, as that term is defined in the GS1 IP Policy. Furthermore, attention is drawn to the possibility that an implementation of one or more features of this Specification may be the subject of a patent or other intellectual property right that does not involve a Necessary Claim. Any such patent or other intellectual property right is not subject to the licensing obligations of GS1. Moreover, the agreement to grant licenses provided under the GS1 IP Policy does not include IP rights and any claims of third parties who were not participants in the Work Group.

Accordingly, GS1 recommends that any organization developing an implementation designed to be in conformance with this Specification should determine whether there are any patents that may encompass a specific implementation that the organization is developing in compliance with the Specification and whether a license under a patent or other intellectual property right is needed. Such a determination of a need for licensing should be made in view of the details of the specific system designed by the organization in consultation with their own patent counsel.

THIS DOCUMENT IS PROVIDED “AS IS” WITH NO WARRANTIES WHATSOEVER, INCLUDING ANY WARRANTY OF MERCHANTABILITY, NONINFRINGEMENT, FITNESS FOR PARTICULAR PURPOSE, OR ANY WARRANTY OTHERWISE ARISING OUT OF THIS SPECIFICATION. GS1 disclaims all liability for any damages arising from use or misuse of this Standard, whether special, indirect, consequential, or compensatory damages, and including liability for infringement of any intellectual property rights, relating to use of information in or reliance upon this document.

GS1 retains the right to make changes to this document at any time, without notice. GS1 makes no warranty for the use of this document and assumes no responsibility for any errors, which may appear in the document, nor does it make a commitment to update the information contained herein.

## Document Summary

Document Item	Current Value
Document Title	GDSN Guide for the FDA GUDID Implementation Guide
Date Last Modified	9 May 2014
Current Document Issue	Issue #1.1
Status	<b>Pending Ratification and IP Review</b>
Document Description	Implementation guide for using the GDSN to populate a UDI database. This version focuses on the U.S. FDA Global Unique Device Identifier Database (GUDID)

## Contributors

Name	Organization
Pete Alvarez	GS1 Global Office
Scott Brown	GS1 US

## Change Log

Issue No.	Date of Change	Changed By	Summary of Change
1	9 September 2013	Pete Alvarez	Merger of sections created by Pete Alvarez (Global Office) and Scott Brown (GS1 U.S.)
2	6 January 2014	Scott Brown	Updated section, GDSN to GUDID Attribute Mapping and Guidance on Populating Attributes per latest FDA GUDID requirements and User Guide
3	8 January 2014		Final Review prior to submitting into the GSMP



Issue No.	Date of Change	Changed By	Summary of Change
4	20 May 2014	Scott Brown	<p>Updated spelling errors, and grammatical errors throughout the document.</p> <p>Updated cover, header, and footer areas to reflect the change in version, and that the version is a Draft and still needs IP review and ratification to occur.</p> <p>Updated Section 3 (page 23), updated the table legend with corrected headers based on the FDA GUDID Guidance document.</p> <p>Updated Section 3 (page 24), updated a note regarding the FDA GUDID Guidance document and the updating of this document to reflect changes in the FDA Documents.</p> <p>Updated Section 3 (pages 25-57), listing of attributes with various changes. Primarily changing the content from the FDA GUDID Guidance documents such as values for the GUDID of Attribute Name Description, Data Entry Notes, Edit Rules After Grace Period, Required?, Data Type &amp; Length, and Entry List of Values (LOV), values for the GDSN of New Attributes, and Guidance. There are also various formatting and spelling changes throughout this section. All changes are in red text and highlighted in yellow. Some changes denote a difference in the FDA GUDID Webtool Guidance and Guidance for the use of HL7 SPL messaging (machine connection to the FDA GUDID). To aid readability and printability, pagination was also changed to allow for each different attribute to start a new page.</p> <p>Updated Section 4 (pages 59-74), various changes such as updating the GUDID attribute name to match previous sections, equivalent GDSN attributes, GDSN definitions, and GDSN Notes have been made, all changes are in red text with yellow highlighting.</p> <p>Updated Section 5 (pages 75-112), various changes such as updating the GUDID attribute name to match previous sections, GUDID code values, and equivalent GDSN Code Values have been made, all changes are in red text with yellow highlighting. There are several code values which have notes as to change request activity with GSMP, when this work completes the document will be updated.</p> <p>Updated Section 5 (pages 113- 161), the Unit of Measure (UoM) section of the code value table was completely redone, specific additions and mapping have been highlighted in red text with yellow highlighting. The table reflects several new columns in use by the GDA GUDID Guidance documents and similar columns in use by GDSN.</p> <p>Updated Section 6 (pages 162-260), listing of attributes with various changes. Primarily changing the content from the FDA GUDID Guidance documents such as values for the GUDID of</p>



Issue No.	Date of Change	Changed By	Summary of Change
4	9 May 2014	Scott Brown	<p>Updated the following sections 3, 4, 5 to align document with the release of the FDA GUDID SPL version 1.2.1 issued on April 16, 2014</p> <ul style="list-style-type: none"> <li>- Added validation guidance for MR Safety Status</li> <li>- Updated UoM list to group codes for clinical size types, highlighted GDSN codes to be removed in the GDSN Major Release, and highlights FDA GUDID Codes (including GDSN Change Request to add)</li> <li>- Added tab containing guidance from the FDA on Premarket Submission Number formats</li> <li>- Added new attributes for the Donation Identification Number, FDA Preferred Term Code (including GDSN Change Request to add)</li> <li>- Noted that the GUDID Attribute Is the device labeled for MRI Safety? Is no longer supported in the SP</li> <li>- Throughout document where the SPL Information is different from the GUDID Web Guideline document, the SPL information has been added in highlighted red text. If either document is amended to match the other, the text will be edited to match the changes. The following are specific changes made: <ul style="list-style-type: none"> <li>- Updated the GUDID Data Element field with the SPL Name for- Support Contact Phone, Support Contact Email, Code (Split into two parts- GMDN Preferred Term Code and a new attribute FDA Preferred Term Code), MRI Safety Status, Size Type Text, Storage and Handling Type, High Value, Low Value, Unit of Measure</li> <li>- Updated the GUDID Definition field with SPL Definition for- Labeler DUNS Number, Secondary DI Number, Contains DI Package, Support Contact Phone, Support Contact Email, Device Exempt from Premarket Submission, Supplement Number, Product Code, Code (Split into two parts- GMDN Preferred Term Code and a new attribute FDA Preferred Term Code), Lot or Batch Number, Manufacturing Date, Serial Number, Expiration Date, Device required to be labeled as containing natural rubber latex or dry natural rubber (21 CFR 801.437), Device labeled as "Not made with natural rubber latex", MRI Safety Status, Size Unit of Measure, Storage and Handling Type, High Value, Low Value, Unit of Measure, Special Storage Conditions</li> <li>- Updated the GUDID Required? Field with the SPL Text for- Package DI Number, Contains DI Package, Package Discontinue Date, Support Contact Phone, Support Contact Email, Code (Split into two parts- GMDN Preferred Term Code and a new attribute FDA Preferred Term Code), MRI Safety Status, Size Type, Size Value, Size Unit of Measure, Size Type Text, Storage and Handling Type, High Value, Low Value, Unit of Measure, Sterilization Method</li> <li>- Updated the GUDID Cardinality field with the SPL Text for- Device Subject to Direct Marking (DM), but Exempt, DM DI Number, Secondary DI Number, Package DI Number, Contains DI Package, Support Contact Phone, Support Contact Email, Device Exempt from Premarket Submission, FDA Premarket Submission Number, Supplement Number, Product Code, Code (Split into two parts- GMDN Preferred Term Code and a new attribute FDA Preferred Term Code), MRI Safety Status, Size Type, Size Value, Size Unit of Measure, Size Type Text, High Value, Low Value, Unit of Measure, Special Storage Conditions, Sterilization Method</li> <li>- Updated the GUDID Data Type field with the SPL Text for- Version or Model Number, Device Description, DI Record Publish Date (Note: date format is different between the Web Portal and the SPL Message),</li> </ul> </li> </ul>

Issue No.	Date of Change	Changed By	Summary of Change
5	9 May 2014	Scott Brown	<p>Corrections to the document sections 3, 4, 5 to correct the following-</p> <ul style="list-style-type: none"> <li>- Corrected the case for the clinical size text code list to be upper case</li> <li>- Corrected the data type of the GDSN attribute fDAMedicalDeviceListing (AVP) to alphanumeric (7characters)</li> <li>- Updated process for Premarket Submissions numbers and their related Supplement numbers. Supplement numbers must be associated with an applicable Premarket Submission Number</li> <li>- Updated the name of the FDA Premarket Submission Number in the FDA GUDID Column on the additional trade item classification agency tab. Enter comment about name and definition changes being requested in GDSN.</li> <li>- Change the attribute used for the FDA GUDID Publish date from effectiveDate to be fDAGUDIDPublishDate (AVP) and a final trading partner dependent deployment of uDIDPublishDate.</li> <li>- Updated the GDSN Notes for the GMDN Preferred Term and Definition attributes"</li> <li>- Corrected the MRI Compatibility codes to be all capitals"</li> <li>- Updated the guidance on the use of the Sterility codes</li> <li>- Added code value of KIT_AND_COMBINATION to denote a TRUE value for both TRUE and COMBINATION"</li> <li>- Corrected GDSN Definitions for the additionalClassificaitonAgency which incorrectly only referenced Premarket Authorization Numbers</li> <li>- Corrected truncated definitions in the packaging type code list</li> <li>- Corrected the MRI Compatibility code for the GDSN from MRI_CONDITIONAL to the correct value from the GDSN Schema of MRI_COMPATIBLE</li> <li>- Corrected missing words in the FDA Required column foe Supplement Number to complete phrase to state "Not Required for Kits."</li> <li>- Updated guidance on how to populate the FDA Premarket Submission Number and its associate Supplement Numbers.</li> <li>- Corrected the name of the Additional Classification header on the Additional Classification Agency code list tab to be "Additional Classification Agency Name"</li> </ul>

# Table of Contents

<b>1. Introduction .....</b>	<b>9</b>
1.1. Purpose of this Document.....	9
1.2. Who Will Use this Document? .....	9
1.3. Prerequisite .....	9
1.3.1. The GS1 Global Company Prefix (GCP) .....	9
1.3.2. The role the Global Trade Item Number (GTIN) and Application Identifiers (AIs) .....	9
1.3.3. Automatic Identification and Data Capture (AIDC) Marking .....	10
1.3.4. The role of Global Location Number (GLN) in UDI .....	10
1.3.5. GDSN Knowledge .....	11
1.4. What is UDI and (G)UDID .....	11
1.5. Mater Data Management and Governance .....	11
1.6. Data Quality .....	12
1.7. Data Management.....	12
1.8. Data Governance .....	14
1.9. Roles and Responsibilities.....	14
<b>2. GDSN Data Flow .....</b>	<b>16</b>
<b>3. GUDID Data Requirements .....</b>	<b>18</b>
<b>4. GDSN to GUDID Mapping .....</b>	<b>53</b>
<b>5. Guidance on Populating Values.....</b>	<b>157</b>
<b>6. References.....</b>	<b>256</b>



# 1. Introduction

## 1.1. Purpose of this Document

The purpose of this document is to explain how to use the Global Data Synchronization Network (GDSN) to securely provide data to a Unique Device Identification (UDI) database. The first version of this implementation guide will focus on the U.S. FDA Global Unique Device Identifier Database (GUDID) requirements since this is the only regulator to issue a UDI rule for medical devices as of this writing. As other regulators introduce UDI regulation this document will be updated as needed.

## 1.2. Who Will Use this Document?

This document is intended primarily for medical device manufacturers who have decided to use GS1 standards to comply with UDI regulation and the GDSN Data Pools who will be required by the medical device customers to provide data on their behalf to a UDI database.

The guidance and GDSN attributes included in this document is based on the published database requirements and GUDID Users' Guide from the U.S. FDA, plus the lessons learnt from the GDSN pilot held as part of the U.S. FDA User Acceptance testing of 2012. This document contains addition guidance on Master Data Management and Governance plus Information Lifecycle Management and Data Quality. This information is intended as general guidance for the purpose of assisting GS1 members. The UDI regulation may contain specific information related to the rule, which in case of conflict supersedes this general guidance.

## 1.3. Prerequisite

It is assumed that the reader is already familiar with the UDI regulation and the database requirements prior to using this implementation guide. For additional information on UDI visit the [GS1 UDI webpage](#) or the website of the specific regulation in question.

Below are a few basics steps the Medical Device manufacturer should consider prior to using the GDSN to register their medical device product data in the appropriate UDI database. The section includes prerequisites for using GS1 standards to implement a UDI regulation.

### 1.3.1. The GS1 Global Company Prefix (GCP)

The GS1 Global Company Prefix is the base component used to create a GS1 Key such as a Global Trade Item Number (GTIN). The GS1 Global Company Prefix is a license to create GS1 Keys and is issued by any one of the GS1 Member Organisations to companies who wish to use the GS1 system.

The GS1 website lists [10 basic steps to bar code implementation](#) and is offered as a guide for getting started. For additional information regarding your GS1 Company Prefix and GS1 standards contact your local [GS1 Member Organisation by visiting the GS1 website](#).

### 1.3.2. Role the Global Trade Item Number (GTIN) and Application Identifiers (AIs)

The Global Trade Item Number (GTIN), as the GS1 trade item "Identification Key", is used to identify medical devices, identifying different product variants and each package configuration to achieve unique and unambiguous identification. The UDI includes at a minimum the "static" portion, a "Device Identifier" (DI), as its "key" to specific device related information stored in a database. The GTIN is the GS1 solution for creating the Device Identifier component of a UDI and accessing medical device information stored in a database.

The Unique Device Identifier also includes a ‘dynamic’ portion, known as the “Production Identifier”, to represent production control information generated as part of the manufacturing process based upon the specific medical device. This Production Identifier (PI) can include, for example, manufacturing date, expiry date, lot number or serial number. GS1 Application Identifiers (AIs) are the GS1 solution for creating the Production Identifier component of a UDI.

**NOTE:** the Production Identifier portion of a UDI is NOT stored in a UDI database.

Additional information regarding the use of the GS1 GTIN and Application Identifiers can be found in the GS1 General Specifications, GS1 Healthcare GTIN Allocation Rules and GS1 UDI support materials (<http://www.gs1.org/healthcare/udi>).

### 1.3.3. Automatic Identification and Data Capture (AIDC) Marking

Marking of the UDI on the medical device packaging (and in some cases the medical device itself), via an Automatic Identification and Data Capture (AIDC) “Data Carrier” technology is a primary requirement of the U.S. FDA UDI ruling. The Data Carrier is the means used to transport the UDI with the medical device and retrieve its unique identification, enabling access to the database stored information. The GS1 System includes specifications for the use of both Bar Code and RFID Data Carriers including (but not limited to) EAN/UPC, GS1-128, GS1 DataMatrix Bar Code symbologies.



Selection of the appropriate GS1 Data Carrier is based upon a number of factors including the UDI to be encoded in the Data Carrier, the distribution channel of the medical device, available space for the Data Carrier among other criteria of the regulation. Additional information and specifications on the selection and use of GS1 Data Carriers can be found in the GS1 General Specifications and GS1 UDI support materials (<http://www.gs1.org/healthcare/udi>).

For additional information on identification of items below the “each” level refer to the GS1 Healthcare GTIN Allocation Rules (<http://www.gs1.org/1/gtinrules/index.php/p=static/t=healthcare>)

### 1.3.4. The role of Global Location Number (GLN) in UDI

The Global Location Number is a 13 digit numeric GS1 standard used to identify locations and legal entities. While the U.S. FDA UDI regulation does not require the use of GLNs in order to comply with the rule, it is required when using the Global Data Synchronisation Network (GDSN) to identify the manufacturer and the data recipients. In addition, the U.S. FDA Global UDI database is identified by GLN 1100001017041 within the GDS Network. This unique identification ensures that there is a single and unique global identification of the U.S. FDA GUDID within the entire GDS Network for all Data Pools to use in the submission and registration of the manufacturer’s medical device product data.

### 1.3.5. GDSN Knowledge

This guide and the information contained within it require the reader to have a basic understanding of the Global Data Synchronisation Network (GDSN). For more information on the GDSN refer to the [GDSN page](#) on the GS1 website or contact a [GS1 member Organisation](#) or a [GDSN certified Data Pool](#).

## 1.4. What is UDI and (G)UDID

The Unique Device Identifier (UDI) is a multinational initiative driven by several medical device regulators with the intention of improving patient safety and healthcare business processes. Each UDI regulation is expected to include a database, which will contain medical device product data. This is referred to as a Unique Device Identifier Database (UDID). For more information in UDI at a global level and how GS1 standards support it refer to the [UDI page on the GS1 website](#). The illustration below provides a basic cross reference between UDI terms and the corresponding GS1 standard.

<b>UDI</b> Unique Device Identification	<b>GS1 Standards</b> Product Identification
<b>UDID</b> Data Elements linked to the Device Identifier	<b>GDSN</b> Attributes mapped to each UDID data element
<b>DI =</b> Device Identifier (DI)	<b>GTIN</b> Global Trade Item Number
<i>Production data is not stored in UDI or GDSN databases</i>	
<b>PI =</b> Production Identifier (PI) (if applicable) Production Identifier data will vary by medical device type and manufacturer current practice.	<b>AI</b> Application Identifiers (AI) <ul style="list-style-type: none"> <li>• Expiration Date AI(17) e.g. 141120</li> <li>• Lot/Batch AI(10) e.g. 1234AB</li> <li>• Serial Number AI(21) e.g. 12345XYZ</li> </ul>
<b>DI + PI = UDI</b>	<b>GTIN -or- GTIN + AI(s) = UDI</b>

Illustration1

The United States Food and Drug Administration is the first regulator to issue an UDI rule. In addition the U.S. FDA operates a database called Global Unique Device Identifier Database (GUDID) designed to store medical device product data. For more information on the U.S. FDA UDI and GUDID and how GS1 standards support it refer to the [UDI page on the GS1 US website](#).

## 1.5. Master Data Management and Governance

One of the most challenging areas related to implementation of the UDI regulation is the Master Data Management and Governance. Master Data Management and Governance (MDM&G) refers to a series of processes and protocols that should exist within an organisation to create, enrich, maintain and publish product information within and outside the enterprise. Equally important is “data quality management,” which is a complementary cycle of activities aimed to ensure that the subject information meets high standards of quality and reliability. In short, the data created by the product manufacturer must meet the requirements of the intended use case. Medical device data which has to comply with UDI regulation is no exception.

Completeness and accuracy of product data is the responsibility of the manufacturer. Each manufacturer should have an internal process to manage the data required by the regulator. This includes:

- data quality checks and procedures
- data management process and policies
- enterprise-wide data governance policies
- roles and responsibilities which outline who has the authority to create, modify and approve the data

GS1 strongly recommends that each manufacturer ensure they have a robust Information MDM&G and data quality process in place as part of their internal data preparation process.

## 1.6. Data Quality

Good data quality is a key ingredient of any efficient supply chain. Having the means to continuously maintain high quality data is not only vital to reducing errors and improving patient safety but also to reducing errors in the supply chain. It is also fundamental to increasing efficiency, reducing costs and positively impacting customer satisfaction.

Good quality data means that all master data is complete, consistent, accurate, time-stamped and industry standards-based. By improving the quality of data, trading partners reduce costs, improve productivity and accelerate speed to market.

For more information on GS1 data quality best practices and recommendations refer to the [Data Quality page on the GS1 website](#)

Some regulators may include specific business and data validations to ensure data quality of the information provided by the manufacturer. Please refer to the specific regulation for more information.

## 1.7. Data Management

Data Management refers to processes and procedures within an enterprise related to lifecycle information management. In relationship to UDI regulation, this refers to product master data and lifecycle management of the related information. The U. S. FDA regulation contains specific data management requirements and recommendations to which a manufacturer must adhere. However, this section contains general guidance as a recommendation to augment the requirements of any regulator. In case of conflict, the regulation supersedes this guidance.

Below are seven basic steps of an information lifecycle management process.

### 1. Create, Import or Receive

The first step is the creation of the product data. This may include gathering information related to the product specifications, raw materials, function, regulatory requirements, and sterilization among other areas. The U.S. FDA GUDID includes a specific list of data requirements and data relationship based on the recommendation from the International Medical Device Regulators Forum (IMDRF), formerly known as the Global Harmonization Task Force plus additional information required by the U.S. FDA. In this step the manufacturer should confirm the core attributes and match against data requirements of the UDI regulation. Sections 3 and 4 of this document contain a listing of the GUDID data requirements and cross reference to GDSN attributes. The U.S. FDA UDI rule and Users Guide supersedes any information found in this document and will always serve as the point of reference for U.S. FDA UDI requirements.

### 2. Enrich and Validate

This step refers to an internal process by which the data created in step one is completed with any missing data, validated for compliance with specific requirements of the UDI regulation and approved. This is a fundamental step in data quality management. GS1 offers general data

quality guidance and best practices based on industry experience including the GS1 Data Quality Protocol. Below are a few basic steps to consider.

- **Completeness:** Is data missing which is needed for that specific product?
- **Accuracy:** Is data precise, correct, and current?
- **Conformity:** Have formatting rules and standards been applied properly?
- **Logic:** Is data valid or conflicting across product classes?
- **Consistency:** Is data consistent across systems for the same field?
- **Integrity:** Are there appropriate data linkages between internal systems?
- **Duplication:** Are there unnecessary representations of the same data?

For specific information regarding data quality and validation requirements of the U.S. Global UDI Database refer to FDA regulation and User Guide.

### 3. Publish and Activate

Once the data is created, enriched, validated and approved it can be published and activated for use. Publication can refer to internal users, catalogs or the GDSN Source Data Pool for data synchronization with external users.

In relationship to UDI, the data should now be ready for registration in the corresponding UDI database, such as the U.S. FDA GUDID. Section two of this document outlines three ways for registering data with the U.S. FDA's GUDID, including how to use a GDSN Data Pool to register the data on behalf of the manufacturer.

### 4. Audit and Evaluate

Part of the information lifecycle management includes routine monitoring to ensure the data is fit for purpose. This is typically an ongoing process, which is part of a continuous data quality management and improvement process. It can be in the form of an actual audit event, but generally it is part of the user feedback process as a result of application of the information. Ideally the Audit is performed against a set of Metrics or Key performance Indicators. Error investigation should include a root cause analysis to determine the cause of the problem and steps to prevent it from re-occurring. Some organizations include a scorecard to report performance and track improvements over time.

### 5. Update and Maintain

The information lifecycle management process should include a step to update information as relevant changes occur in any part of the master data. This applies to information about the product as well as well as the organization. This step should include notification of the change to the data owner for approval.

### 6. Inactivate and Archive

As information is obsoleted and purged, it should be removed from active use. This may include a flag to indicate that a particular data element is inactive and is no longer used, but it is not removed from the listing. This is a very relevant step in UDI regulation, which requires data which has been made inactive to be permanently stored in a UDI database. In general master data management, the data element can be archived from the internal active database. The determination of which action applies usually depends on particular use case for which the data is intended, such as UDI regulation.

### 7. Purge

Generally speaking outdated information should be deleted from systems where it has been stored as part of the publication process. This should include the generation of a Purge List, which should be provided to the internal data owners and users. In some cases this may include the approval of the purge by the data owner.



The U.S. FDA UDI rule includes specific requirements regarding the information lifecycle management, which may supersede guidance found in this document. For additional information refer to the U.S. FDA GUDID User's Guide.

## 1.8. Data Governance

Data governance relates to an enterprise wide process which includes decision authority, policy and issue escalation. An enterprise wide Data Governance process should include data management, data quality, data policies and risk management and executive sponsorship. The process should ensure that certain data assets are formally recognized and managed throughout the organization.

Data Governance is a critical component of Master Data Management and especially important to the accuracy of the data requirements of a UDI regulation. Each manufacturer is responsible for submitting and maintaining their data in the UDI database.

Data Governance should include the decision rights and accountability of the key pillars:

- **Executive:** Internal sponsors of the Master Data Management process within an organization executive management.
- **Legal / Legislative:** Internal sponsors responsible for the representation of regulatory affairs as it relates to information management and publication in both internal and external systems and databases. This includes legal compliance, legislative and regulatory requirements. This is especially important with UDI regulation.
- **Administrative:** Internal function responsible for the maintenance of the Master Data. The function can be either centralized or decentralized.

Refer to the Roles and Responsibilities section of this document for more information in functional responsibilities.

## 1.9. Roles and Responsibilities

The Data Governance policies should include clear determination, documentation and enterprise wide education of the Roles and Responsibilities of each function across the information supply chain. This should include a determination of how data is managed within an organization and the roles associated with the process. Generally speaking, there are two overarching models, centralized or decentralized. Most commonly, the responsibilities are spread across an entire organization ranging from manufacturing, to product management to regulatory affairs. Which model applies to a particular organization depends on many factors, such as organizational structure, size and policies related to corporate versus division autonomy and perhaps even legal incorporation of the various divisions, which make up the organization.

There are many models for establishing and documenting Roles and Responsibilities. The first step should be to determine if your organization has a corporate philosophy or policy for assigning roles and responsibilities for information lifecycle management. If not, a basic place to start might be the RACI model.

- **R = Responsible** - owns the project, problem or task. The person responsible for doing the work to achieve the task
- **A = to whom the R is Accountable** - who must sign-off (approve) work before it is effective
- **C = to be Consulted** – has information and/or capability necessary to complete the work
- **I = to be Informed** – must be notified of results, need not be consulted

This simple yet effective model can be applied in any size company. In large organizations, which include divisions in various parts of the world the roles and responsibilities are usually

managed in decentralized manner. Conversely, in a small organisation everyone involved in the information management supply chain may be located in a single location. The level of specificity depends on the granularity needed in order for the Master Data Management and Governance process to be effective and for it to meet its intended purpose. For the purpose of UDI regulation, the internal Regulatory Affairs function should be consulted as well.

## 2. GDSN Data Flow

This section is specific to the U.S. FDA GUDID as it is the first UDI database. This section will be updated as other regulators introduce UDI regulation.

### Options for registering data in the FDA GUDID:

1. Manual data entry via the Web based tool. This refers to a web portal provided by the U.S. FDA to register data directly in their GUDI. The portal provides a means for the medical device manufacturer to enter and update their data manually directly in their database.
2. Bulk data registration direct from a manufacturer's internal application using the HL7 standard. This refers to a machine to machine automated method of registering data. It requires the use of the Standard Product Labelling standard from HL7. This provides the means for a manufacturer to register data directly from an internal application, such as an ERP, to the GUDID. The manufacturer must convert their internal data record into the HL7 SPL standard.
3. GDSN certified Data Pools can register data on behalf of the manufacturers using the HL7 Structured Product Labeling (SPL) standard. The manufacturer will need list their data pool as their data provider when they create their "Labeler" profile with the FDA. GS1 successfully tested this capability with 8 manufacturers with the support of 1Worldsync and GHX in 2012 during the FDA's user acceptance testing.

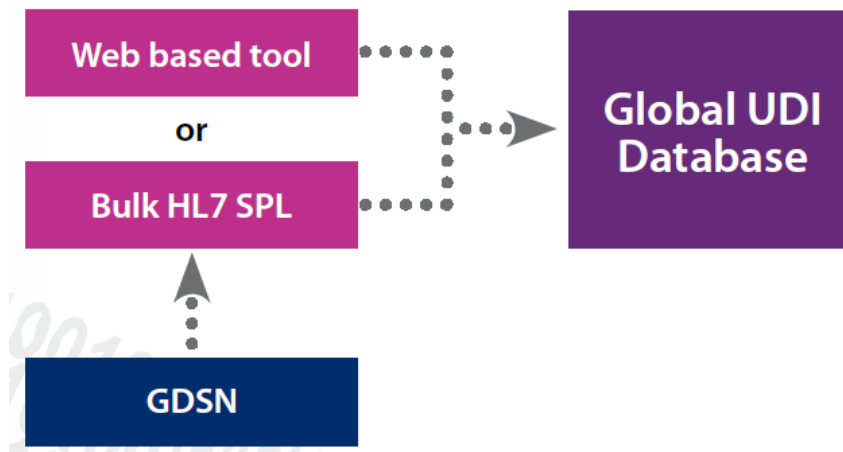


Illustration 2

The GDSN is an Internet-based, interconnected, network of interoperable data pools and a Global Registry, the GS1 Global Registry® that enables companies around the world to exchange accurate, standardised and synchronised supply chain data with their trading partners. The Global Data Synchronisation Network (GDSN) enables manufacturers, distributors and providers to share accurate product information electronically. In addition to receiving the initial product data, the customer can receive product update notifications automatically from the supplier.

The GDSN is an attractive option for manufacturers who also need to provide product master data to providers, GPOs and distributors since it allows them to provide the right data to the right party with a single connection, as illustrated below.



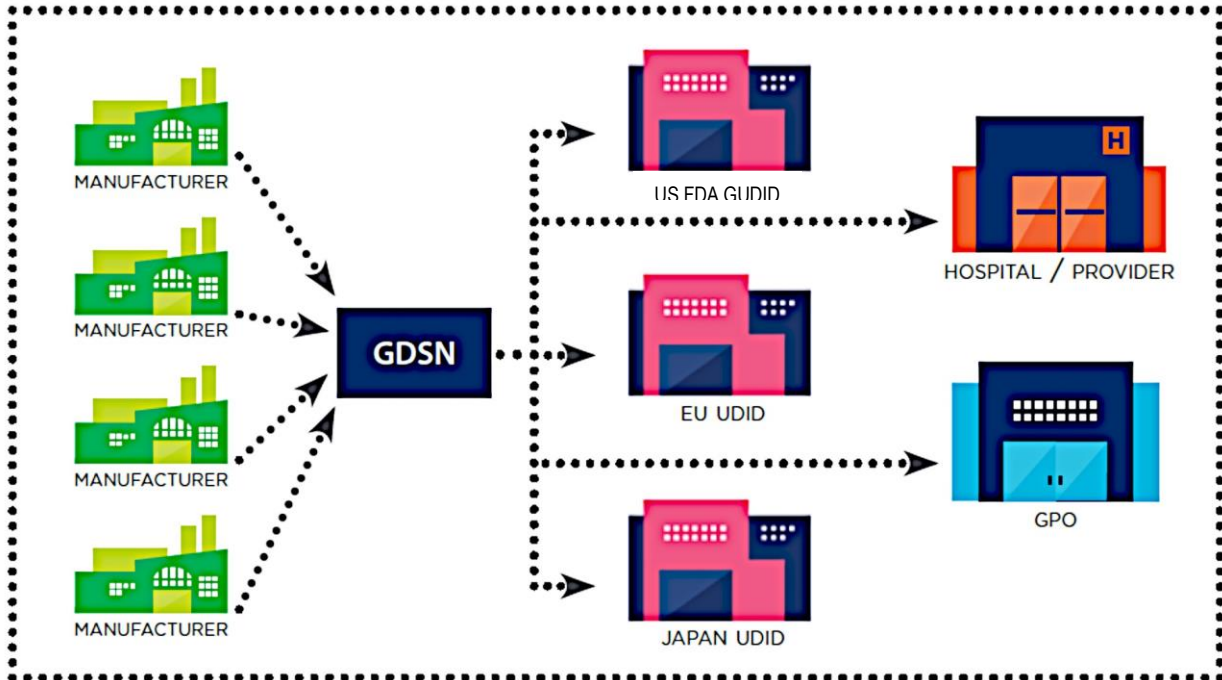


Illustration 3

Regulators are working together via the International Medical Device Regulators Forum (IMDRF) to align as much of their requirements as possible. However, each regulator will probably have a specific and distinct set of data requirements. This means that manufacturers will need to maintain separate data records for each UDI regulator’s database. Additionally, they will need to establish separate connections, or methods, of registering their product data in the particular UDI database. The GDSN provides a means for any manufacturer of any size, to provide data to all UDI databases and their customers (hospitals, distributors, wholesalers, GPOs) simultaneously, with a single connection.

Below are the high-level steps of the data flow from the manufacturer to the GUDID when using a GDSN Data Pool.

1. The manufacturer prepares data required by the Global UDI Database
2. The manufacturer provides GUDID data to their GDSN Data Pool of choice
3. The GDSN Data Pool converts the data provided by the manufacturer to the HL7 SPL format (refer to the GUDID User Manual for information)
4. The GDSN Data Pool registers the manufacturer’s product data using the HL7 SPL format in the GUDID
5. The GDSN Data Pool confirms the registration with the Manufacturer, once a confirmation from the GUDID is received by the GDSN Data Pool.

The GDSN provides a secure and easy way for manufacturers to register their product data with any UDI database, anywhere in the world, via a single connection. Refer to the GDSN website for a list of GDSN certified Data Pools <http://www.gs1.org/gdsn>

### 3. GUDID Data Requirements

The Device Identifier (DI) is the primary key in the UDI database and will be linked to other product data elements. Manufacturers will be responsible for submitting and maintaining their own data in the database. The U.S. FDA Global UDI Database (GUDID) will not contain the Production Identifiers, i.e. Expiration Date, Batch/Lot Number, Serial Number or others.

*“The core elements are the minimum elements needed to identify a medical device through distribution and use. Regional or National UDID may contain additional elements; however, these additional elements should be kept to a minimum” – International Medical Device Regulators Forum (IMDRF), UDI System for Medical Devices*

The Global Unique Device Identification Database (GUDID) has a set of attributes for population of information about a medical device. These attributes are of various types (Boolean, Code List, Text, etc.) and if it is “Required” or “Not Required”. The specifics of each attribute varies based upon the information requested by the attribute’s definition and the type of device being described.

The table below provides a list of the GUDID attributes and their particulars as current at the time of the creation of this document as provided by the FDA GUDID Guidance documents. While every effort is made to keep this document up to date, the official list of attributes and particulars is the responsibility and jurisdiction of the FDA. A website link to the official list is provided in the reference section of this document. Users of this document are encouraged to review and become familiar with the official list of attributes and particulars as listed on the FDA’s websites. The table uses the headers as defined below.

Header	Definition
<b>Data Element</b>	The name of the element being requested.
<b>Description</b>	Text defining the element.
<b>Data Entry Notes</b>	How the entry is to be accomplished. The primary focus of the guidance is primarily written with a web interface user in mind. For a machine to machine user, the notes will have different meaning and be described in the guidance later in this document.
<b>Edit (Editing of entered data is allowed) Rules after Grace Period</b>	Once published on the FDA GUDID public facing website for the first time, the user will have a 7-day grace period within which changes can be made. This field states what editing can be accomplished after the grace period expires.
<b>Required?</b>	Is this data element required to be populated by the FDA? 0 in the first position signifies not required, 1 in the first position signifies required, * after 2 periods signifies multiple occurrences/repeatability, and a number after 2 periods signifies single occurrence/non-repeatability
<b>Data Type &amp; Length</b>	The type of value for the element (Boolean, Text, Code List, etc) including how many characters are available for population.
<b>Entry List of Values (LOV)</b>	This is a list of values which can be provided for code list attributes
<b>New DI Trigger?</b>	Indicator signifying if a change to this data element would trigger a new Device Identifier to be created. In GS1 Standards, this indicates if a new GTIN should be created due to a change in the value for this element.
<b>Public/ Private Status</b>	Indicator signifying if this element will be posted on the FDA GUDID public facing website (PUBLIC) or for FDA consumption only (PRIVATE)

## Document reference:

- The FDA term GS1 14-digit numeric value is equal to a GTIN.
- The FDA term “Primary DI” in GS-speak would be the primary device GTIN. For example a DI 101 is the Primary GTIN and DIs 201 and 301 would be the packaging levels

**Note:** FDA published an updated SPL Guideline on April 16, 2014 and an updated Appendix B on May 7, 2014. Changes have been highlighted in yellow throughout this document. Once all documentation is changed and ratified, the highlighting will be removed and this document will change as well.

Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
When a GUDID attribute appears on the medical device package/label, the values submitted to the GUDID should match the value on the label.								
<b>Device Information</b>								
<b>Device Identifier (DI) Information</b>								
<b>Issuing Agency</b>	Organization accredited by FDA to operate a system for the issuance of UDIs.	Choose a value from the drop down <b>LOV</b> .	None (NO edit, add, or delete are allowed)	Required	NA	GS1; HIBCC; ICCBBA	YES	Public
<b>Primary DI Number</b>	An identifier that is the main (primary) lookup for a medical device and meets the requirements to uniquely identify a device through its distribution and use. The primary DI number will be located on the base package, which is the lowest package level of a medical device containing a full UDI. For medical devices without packaging, the primary DI number and full UDI may be on the device itself.	Enter the Device Identifier (DI) Number. Data type and field length are determined by the individual Issuing Agency structure.  GS1: Numeric (Num.), with 14 digits HIBCC: Alphanumeric (Alphanum.), with 6-23 characters ICCBBA: Alphanumeric, with 10 or 16 characters	None (NO edit, add, or delete are allowed)	Required	Type: Num. or Alphanum.  Length: min-6, max-23*  *defined by Issuing Agency structure.	N/A	YES	Public
<b>Device Count</b>	Number of medical devices in the base package.	Enter the number of devices.  Example: Base Package = Box of 100 gloves; Primary DI = 101; Device Count = 100.	None (NO edit, add, or delete are allowed)	Required	Type: Num.  Length: 7	N/A	YES	Public

Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
<b>Unit of Use DI Number</b>	An identifier assigned to an individual medical device when a UDI is not labeled on the individual device at the level of its unit of use. Its purpose is to associate the use of a device to/on a patient.	<p>Enter the Unit of Use DI Number.</p> <p>Unit of Use DI is an identifier used by hospital staff and Materials Management to account for a single device when the UDI is labeled on a higher level of packaging. The Unit of Use DI does not appear on the label.</p> <p>Data type and field length are determined by the individual Issuing Agency structure.</p> <p>GS1: Numeric (Num.), with 14 digits  HIBCC: Alphanumeric (Alphanum.), with 6-23 characters  ICCBBA: Alphanumeric, with 10 or 16 characters</p> <p>If Device Count = 1, cannot add Unit of Use DI Number.</p>	<p>Edit (Editing of entered data is allowed)</p>	<p>Conditionally Required*</p> <p>*If Device Count &gt;1.</p>	<p>Type: Num. or Alphanum.</p> <p>Length: min-6, max-23*</p> <p>*defined by Issuing Agency structure.</p>	N/A	NO	Public
<b>Labeler DUNS Number</b>	Business number issued by Dun & Bradstreet (D&B) that is used to associate the Labeler	<p>*Choose appropriate DUNS Number from drop down LOV.</p> <p>To ensure data</p>	<p>Edit (Editing of entered data is allowed)*</p> <p>*Other Labeler DUNS listed to your GUDID</p>	Required	NA	Labeler DUNS LOV	NO	Private



Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
	(Company) name and address to a given version of model of a device in GUDID.	consistency for the GUDID, DUNS number submitted to the GUDID should associate to the company name that appears on the device label; ideally the address associated with the DUNS number should also match the address on the device label, but since address is not displayed to the GUDID public user, this is not a requirement for data consistency. All edits to information connected to the Labeler DUNS Number must be done through Dun & Bradstreet. No edits of DUNS information will be permitted in the GUDID. "	account can be selected. No Edit (Editing of entered data is allowed)s of DUNS info will be permitted.					



Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
<b>Company Name</b>	Company name associated with the labeler DUNS Number entered in the DI Record.	Auto populated based on the Labeler DUNS Number  The labeler company name submitted to the GUDID should match the company name on the device label.	NA (data element is not able to be changed directly; most are 'auto-populated' fields whose information depends on another data element)	Auto Populated	NA	NA	N/A	Public
<b>Company Physical Address</b>	Company physical address associated with the labeler DUNS Number entered in the DI Record.	Auto populated based on the Labeler DUNS Number  Ideally, this address should match the labeler address as shown on the device label but since this data element is not be displayed to the GUDID public user, this is not a requirement for data consistency.	NA (data element is not able to be changed directly; most are 'auto-populated' fields whose information depends on another data element)	Auto Populated	NA	NA	N/A	Private
<b>Brand Name</b>	The Proprietary/Trade/Brand name of the medical device as used in device labeling or in the catalog. This information may 1) be on a label attached to a durable device, 2) be on a package of a disposable device, or 3) appear in labeling materials of an	Enter the Brand Name.  Only symbols, ® and ™ will be supported for the current production release of GUDID. NOTE: per Edit Rules, you will not be able to change ® or ™ (if entered) after the Grace Period. Enter NA if the device does not	None (NO edit, add, or delete are allowed)	Required	Type: Alphanum.  Length: 80	NA	YES	Public

Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
	implantable device. The brand name is the name that is typically registered with USPTO and have the ® and/or ™ symbol.	have a Brand Name.						
Version or Model Number	The version or model found on the device label or accompanying packaging used to identify a category or design of a device. The version or model identifies all devices that have specifications, performance, size, and composition within limits set by the labeler.	Enter the Version or Model.  Version/Model can be any distinguishing string of letters and/or numbers. Catalog Number can be entered if device does not currently have a Version or Model. If the device does not have a version, model or catalog number, enter a concept that can be used to identify all devices that have specifications, performance, size, and composition within limits set by the labeler.	None (NO edit, add, or delete are allowed)	Required	Type: Alphanum.  Length: 40	NA	YES	Public
Catalog Number	The catalog, reference, or product number found on the device label or accompanying packaging to identify a particular product.	Enter the Catalog or Reference Number.  Catalog/Reference number can also serve as Version/Model if it represents the devices that have specifications,	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)	Optional	Type: Alphanum.  Length: 40	NA	NO	Public



Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
		performance, size, and composition within limits set by the labeler.						
<b>Device Description (max 2000 characters)</b>	Additional relevant information about the device that is not already captured as a distinct GUDID data attribute.	Enter device description.  Device description should include any description found on the device label to support user comparison of the device label to the GUDID device record. Otherwise, include any additional description or text found in the device labeling.	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)	Optional	Type: Alphanum.  Length: 2000	NA	NO	Public
<b>Commercial Distribution</b>								
<b>DI Record Publish Date (mm/dd/yyyy)</b>	Indicates the date the DI Record is published and available via Public Search.	Choose date from calendar or manually enter date in new format (yyyy-mm-dd).  This date determines the Grace Period; the 7 calendar days start the day after the DI Record Publish Date. This date should be set in the future to allow time to ensure accurate data entry. We recommend you set this date in the future, but 7 days prior to any compliance	None (NO edit, add, or delete are allowed)	Required	Type: Num. (date format)  Length: 10	NA	NO	Public



Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
		deadline.						
<b>Commercial Distribution End Date (mm/dd/yyyy)</b>	Indicates the date the device is no longer held or offered for sale. See 21 CFR 807.3(b) for exceptions. The device may or may not still be available for purchase in the marketplace.	Choose date from calendar or manually enter date in new format (yyyy-mm-dd).	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)	Optional	Type: Num. (date format)  Length: 10	NA	NO	Public
<b>Commercial Distribution Status</b>	Indicates whether the device is in commercial distribution as defined under 21 CFR 807.3(b).	Auto populated based on Commercial Distribution End Date. If no Commercial Distribution End Date is entered, the status is 'In Commercial Distribution'	NA (data element is not able to be changed directly; most are 'auto-populated' fields whose information depends on another data element)	Auto Populated	NA	In Commercial Distribution; Not in Commercial Distribution	NO	Public
<b>Alternative or Additional Identifiers</b>								
Direct Marking (DM)								
Direct Marking (DM) data elements only apply to devices subject to 21 CFR 801.45.								
<b>Device Subject to Direct Marking (DM), but Exempt</b>	The device is exempt from Direct Marking requirements under 21 CFR 801.45.	Select checkbox if appropriate.  Labeler should select the checkbox "Device Subject to Direct Marking (DM), but Exempt" only if the device: (1) is	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is	Conditionally Required*  *If device is subject to 801.45	Type: Boolean	NA	NO	Public

Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
		intended to be used more than once and (2) is intended to be reprocessed before each use, but also (3) meets any one of the exception criteria outlined under 21 CFR 801.45(d). If the device is not required to be directly marked under 21 CFR 801.45(a), then this box should not be checked.	allowed)					
<b>DM DI Different from Primary DI</b>	Indicates that the DM DI Number is different than the Primary DI Number.	Select checkbox if appropriate.	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)	Conditionally Required*  *If device is subject to 801.45	Type: Boolean	NA	NO	Public
<b>DM DI Number</b>	An identifier that is marked directly on the medical device and is different than the Primary DI Number; only applicable to devices subject to Direct Marking requirements under 21 CFR 801.45.	Enter Direct Marking DI Number. Data type and field length are determined by the individual Issuing Agency structure.  GS1: Numeric (Num.), with 14 digits HIBCC: Alphanumeric (Alphanum.), with 6-23 characters ICCBBA:	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)	Conditionally Required*  *If device subject to 801.45 and 'DM DI Different from Primary DI' is checked	Type: Num. or Alphanum.  Length: min-6, max-23*  *defined by Issuing Agency structure.	NA	NO	Public



Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
		Alphanumeric, with 10 or 16 characters						
<b>Secondary DI</b>								
<b>Secondary DI Issuing Agency</b>	Name of Secondary DI Issuing agency.	Choose a value from the drop down LOV.	None (NO edit, add, or delete are allowed)	Optional	NA	GS1; HIBCC; ICCBBA; NDC/NHRIC	NO	Public
<b>Secondary DI Number</b>	<p>Enter Secondary DI Number. If your product is labeled with a UDI and barcode from more than one issuing agency (for regulatory or marketing reasons), you must choose one issuing agency system as the Primary DI and enter the other issuing agency information here, as a Secondary DI.</p> <p>Data type and field length are determined by the individual Issuing Agency structure.</p> <p>GS1: Numeric (Num.), with 14 digits            HIBCC: Alphanumeric (Alphanum.), with 6-23 characters</p>	None (NO edit, add, or delete are allowed)	Optional	<p>Type: Num. or Alphanum.</p> <p>Length: min-6, max-23*</p> <p>*defined by Issuing Agency structure.</p>	NA	<p>Enter Secondary DI Number. If your product is labeled with a UDI and barcode from more than one issuing agency (for regulatory or marketing reasons), you must choose one issuing agency system as the Primary DI and enter the other issuing agency information here, as a Secondary DI.</p> <p>Data type and field length are determined by the individual Issuing Agency structure.</p> <p>GS1: Numeric (Num.), with 14 digits            HIBCC: Alphanumeric (Alphanum.), with 6-23 characters            ICCBBA: Alphanumeric, with</p>	NO	Public

Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
	ICCBBA: Alphanumeric, with 10 or 16 characters					10 or 16 characters		
<b>Package DI</b>	Every device package shall bear a UDI, 21 CFR 801.20(a)(2). Package DIs do not need their own DI record; instead package information should be entered in the Package DI section of the Primary DI record for that device. According to 21 CFR 801.3, a package is defined as a fixed quantity of a particular version or model of a device.							
<b>Package DI Number</b>	A device identifier for the package configuration that contains multiple units of the base package (does not include shipping containers).	Enter Package DI Number. Data type and field length are determined by the individual Issuing Agency structure.  GS1: Numeric (Num.), with 14 digits HIBCC: Alphanumeric (Alphanum.), with 6-23 characters ICCBBA: Alphanumeric, with 10 or 16 characters  Examples: Box of Gloves = DI 101 4 Boxes of Gloves (DI 101) in a Carton = Package DI 201 (the UDI on the Carton) 5 Cartons (Pkg DI 201) in a Case = Package DI 301 (the UDI on the Case)	Add (Addition of new data is allowed)	Conditionally Required*  *If device is available in higher levels of packaging	Type: Num. or Alphanum.  Length: min-6, max-23*  *defined by Issuing Agency structure.	NA	NO	Public



Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
		10 Boxes of Gloves (DI 101) in a Carton = Package DI 202 (the UDI on the Carton).						
Quantity per Package	The number of packages with the same Primary DI or Package DI within a given packaging configuration.	Enter the number of devices per package. The quantity of a package configuration must be >1.  Examples: Package – Carton, Pkg DI 201 contains 4 boxes of DI 101; the quantity per package is 4. Package – Case, Pkg DI 301 contains 5 cartons of Pkg DI 201; the quantity per package is 5. Package – Carton, Pkg DI 202 contains 10 boxes of DI 101; the quantity per package is 10.	Add (Addition of new data is allowed)	Conditionally Required*  *If Package DI is entered	Type: Num.  Length: 9	NA	NO	Public

Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
<b>Contains DI Package</b>	The Primary DI for the base package or the Package DI for any lower level package configuration contained within a given package configuration.	Choose a value from the drop down LOV.  Examples: Package DI 201 (Carton) contains base package DI 101. Package DI 202 (Carton) contains base package DI 101. Package DI 301 contains lower level Package DI 201 (Carton).	Add (Addition of new data is allowed)	Conditionally Required*  *If Package DI is entered	NA	DI numbers; base package and all lower levels of packaging	NO	Public
<b>Package Type</b>	Text to describe the outer packaging of the product and enables users to understand higher level packaging configurations.	Enter name or description of package. This field is free text. There is no implied definition or standard quantity to any package name.	Add (Addition of new data is allowed)	Optional	Type: Alphanum.  Length: 20	NA	NO	Private
<b>Package Discontinue Date</b>	Indicates the date this particular package configuration is discontinued by the labeler.	Choose date from calendar or manually enter in format (yyyy-mm-dd).  Discontinuation of a package is directly related to the discontinuation of the primary DI of the base package. However, a package can also be discontinued without the discontinuation of	Add (Addition of new data is allowed)	Conditionally Required*  *If Package DI Number and Commercial Distribution End Date are entered, must also enter Package Discontinue Date	Type: Num. (date format)  Length: 10	NA	NO	Public



Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
		the base package.						
<b>Package Status</b>	Indicates whether the package is in commercial distribution as defined under 21 CFR 807.3(b).	Auto populated based on Package Discontinue Date. If Package DI and related elements are entered and no Package Distribution End Date is entered, the status is 'In Commercial Distribution.'	NA (data element is not able to be changed directly; most are 'auto-populated' fields whose information depends on another data element)	Auto Populated	NA	In Commercial Distribution; Not in Commercial Distribution	NO	Public
<b>Support Customer Contact</b>								
<b>Support Contact Phone</b>  <b>SPL Name: "Customer Contact Phone"</b>	Phone number for the support contact.  SPL Definition: "Phone number for the Customer contact; to be used by patients and consumers for device-related questions."	Enter 10 digit North American number. For international numbers, start with "+" Does not require the use of () or -, but can enter these symbols.	Can edit, add, or delete after Grace Period.	1..* Required if support contact information is entered  SPL Text: "1..1 Conditionally Required* *ONLY required if Customer Contact Phone is entered"	Numeric, 20 (10)  SPL Text: "Alphanumeric"	N/A	NO	Public
<b>Support Customer Contact Email</b>  <b>SPL Name:</b>	Email for the Customer contact; to be used by patients and consumers for device-related	Enter email address.  This email address could be the same one that appears	Add (Addition of new data is allowed) Delete (Deletion of entered data	Conditionally Required*  *ONLY required if	Type: Alphanum.  Length: 100	NA	NO	Public



Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
"Customer Contact Email"	questions.	on the device labeling or the company website. Labelers can identify a Customer Contact email and a Customer Contact phone number for each device record.  If a phone number is entered and you don't have a Customer Contact email, please enter 'xxx@xxx.xxx'	is allowed) Edit (Editing of entered data is allowed)	Customer Contact Email is entered				
<b>Device Status</b>								
<b>Human Cell, Tissue or Cellular or Tissue-Based Product (HCT/P)</b>	Indicates that the product contains or consists of human cells or tissues that are intended for implantation, transplantation, infusion, or transfer into a human recipient as defined under 21 CFR 1271.3.	Select checkbox if DI record is for a product defined under 21 CFR 1271.3  If checked, the labeler must assign and label each HCT/P device with a distinct identification code, per 21 CFR 1271.290(c). The distinct identification code may take the form of a Donation Identification Number (DIN), serial number, lot number, or a combination of these production identifiers (PIs). Labelers of HCT/Ps regulated	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)	Optional  If no data is provided, 'No' is stored	Type: Boolean	NA	NO	Public

Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
		as medical devices should select the appropriate type of PI that appears on the label of the device.						
<b>Kit</b>	Indicates that the device is a convenience, combination, in vitro diagnostic (IVD), or medical procedure kit. Kits are a collection of products, including medical devices, that are packaged together to achieve a common intended use and is being distributed as a medical device.	Select checkbox if DI record is for a kit. Do not check if the device is a constituent part of a kit.	None (NO edit, add, or delete are allowed)	Optional  If no data is provided, 'No' is stored	Type: Boolean	NA	YES	Public
<b>Combination Product</b>	Indicates that the product is comprised of two or more regulated products that are physically, chemically, or otherwise combined or mixed and produced as a single entity; packaged	Select checkbox if DI record is for a combination product. Do not check if the device is a constituent part of a combination product.	None (NO edit, add, or delete are allowed)	Optional  If no data is provided, 'No' is stored	Type: Boolean	NA	YES	Public

Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
	together as a single package; or packaged separately for the intended use together as defined under 21 CFR 3.2(e). At least one of the products in the combination product must be a device in this case.							
<b>Premarket</b>								
<b>Device Exempt from Premarket Submission</b>	<p>Device is exempt from FDA Premarket regulations; or a preamendment device.</p> <p><b>SPL Definition:</b> "FDA Premarket submission is not required for this device."</p>	<p>Select checkbox if FDA has by regulation exempted this device from premarket submission requirements; or for preamendment devices that are not subject to premarket submission requirements.</p> <p>If left unselected, a 'No' is stored and a Premarket Submission Number should be entered below.</p>	None (NO edit, add, or delete are allowed)	Conditionally Required*	Type: Boolean	NA	NO	Public

Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
<b>FDA Premarket Submission Number</b>	Number associated with the regulatory decision regarding the applicant's legal right to market a medical device for the following submission types: 510(k), PMA, PDP, HDE, BLA, and NDA.	<p>Enter current FDA Premarket Submission Number(s). Each DI record represents a version or model of a device. For each DI record, you must submit the original premarket authorization number and the supplement number through which you obtained approval or clearance for the version or model identified in the DI record, as required by 830.310(b)(11). FDA Premarket Numbers should be verified with the FDA PMA or 510(k) database to make sure the Number represents the subject of the device record. Device records should be updated with additional numbers in the future, as needed.</p> <p>Example: PMA #123456 should be entered as 'P123456.'</p>	Add (Addition of new data is allowed)	<p>Conditionally Required*</p> <p>*Premarket Submission Number OR exempt status fulfills regulatory requirement.</p>	<p>Type: Alphanumeric.</p> <p>Length: 8</p>	NA	NO	Public



Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
Supplement Number	Number assigned by FDA to a supplemental application for approval of a change in a medical device with an approved PMA, HDE, or PDP.	Enter all valid Supplement Numbers. Each DI record represents a version or model of a device. For each DI record, you must submit the original premarket authorization number and the supplement number through which you obtained approval for the version or model identified in that DI record, as required by 830.310(b)(11). Although not all PMA supplements are applicable to a given model or version, if FDA approves a subsequent supplement applicable to that version or model, the GUDID DI record must be updated with that supplement number, in accordance with 21 CFR 830.330(b). 30 day notice supplements should be submitted ONLY if the 30 day notice impacts the device design specifications, or	Add (Addition of new data is allowed)	Conditionally Required*  *Premarket Submission Number OR exempt status fulfills regulatory requirement.	Type: Num.  Length: 4	NA	NO	Public

Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
		performance of the finished devices. Do not enter alpha characters. Example: Supplement 4 should be entered as 004.						
<b>FDA Product Code</b>								
<b>Product Code</b>	Classification for devices issued by the FDA.	Enter all applicable Product Codes, three-letter code. For all PMA and 510k devices, Product Codes are assigned in the FDA approval or clearance letter, respectively. For Class I and exempt devices, the device Product Code may be self-identified.	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)	Conditionally Required*  *Unless device is a kit or IVD with a BL premarket submission number	Type: Alpha Length: 3	FDA Product Code list	NO	Public
<b>Product Code Name</b>	Name associated with the three-letter Product Code.	Auto populated based on 3-letter Product Code	NA (data element is not able to be changed directly; most are 'auto-populated' fields whose information depends on another data element)	Auto Populated	NA	NA	NO	Public
<b>FDA Listing</b>								
<b>FDA Listing Number</b>	Number assigned by FDA during Registration and Listing to all devices in commercial	Enter all relevant listing numbers that enable the labeler to commercially distribute the given version or model of device.	Add (Addition of new data is allowed)	Conditionally Required*  *Unless device is an HCT/P, kit or IVD with	Type: Alphanum. Length: 7	NA	NO	Private



Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
	distribution, regardless of pre-market authorization requirements per 21 CFR 807.28(f).	Listing number is optional for HCT/P devices, Kits and IVDs with a BLA premarket number.		a BL premarket submission number				
<b>GMDN</b>								
<b>Code</b>		Enter all applicable GMDN Preferred Term Codes or FDA PT Codes. Each device record must have at least one assigned GMDN Code/FDA PT Code; DI records are allowed >1 GMDN Code/FDA PT Code, if necessary. Must enter GMDN Code OR FDA PT Code, please don't enter both codes for the same GMDN Name and Definition. The FDA PT Codes can be found in the Find FDA PT Code Module on the GUDID website. For GMDN Codes: Enter only the 5-digit number, omit the 'P'. For FDA PT Codes: Enter the 4-letter code.	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)	Required	Type: Num. Length: 5	NA	NO	Private
SPL Name - FDA Preferred Term Code	SPL Text: "Unique four-character value assigned by the			SPL Text: "1..* Required - either GMDN PT Code or FDA PT	SPL Text: "Alpha, 4"	SPL Text: "FDA DB"		

Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
	FDA to indicate a GMDN Preferred Term without exposing the GMDN PT Code."			Code"				
<b>Name</b>	Name of the common device type associated with the GMDN Preferred Term Code/FDA PT Code.	Auto populated based on GMDN Preferred Term Code/FDA PT Code.	NA (data element is not able to be changed directly; most are 'auto-populated' fields whose information depends on another data element)	Auto Populated	NA	NA	NO	Public
<b>Definition</b>	Definition of the common device type associated with the GMDN Preferred Term Code/FDA PT Code.	Auto populated based on GMDN Preferred Term Code/FDA PT Code.	NA (data element is not able to be changed directly; most are 'auto-populated' fields whose information depends on another data element)	Auto Populated	NA	NA	NO	Public
<b>Device Characteristics</b>								
<b>For Single-Use</b>	Choose Yes/No from the drop down list.	None (NO edit, add, or delete are allowed)	Required	Type: Boolean	Choose Yes/No from the drop down list.	Yes/No	YES	Public
<b>Production Identifier(s) on Label</b>								



Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
<b>Lot or Batch Number</b>	Indicates the device is managed by lot or batch number. This number can be found on the device label or packaging. Lot or Batch means one finished device or more that consist of a single type, model, class, size, composition, or software version that are manufactured under essentially the same conditions and that are intended to have uniform characteristics and quality within specified limits.	Choose Yes/No from the drop down list.  For stand-alone software, select Yes to indicate that the software version number will be represented as a Lot or Batch number	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)	Required	Type: Boolean	Yes/No	NO	Public
<b>Manufacturing Date</b>	Indicates the device is managed by date of manufacture; the date a specific device was manufactured.	Choose Yes/No from the drop down list.	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)	Required	Type: Boolean	Yes/No	NO	Public
<b>Serial Number</b>	Indicates the device is managed by serial number. This number can be found on the device label or packaging. The serial number is assigned by the labeler and should	Choose Yes/No from the drop down list.	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)	Required	Type: Boolean	Yes/No	NO	Public

Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
	be specific to each device.							
<b>Expiration Date</b>	Indicates the device is managed by expiration date; the date by which the label of a device states that the device must or should be used.	Choose Yes/No from the drop down list.	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)	Required	Type: Boolean	Yes/No	NO	Public
<b>Donation Identification Number</b>	Indicates the device is managed by a Donation Identification Number. This number can be found on the device label or packaging. The Donation Identification Number is applicable to devices that are also regulated as HCT/Ps and is a number that is assigned to each donation.	Choose Yes/No from the drop down list.  This PI is only applicable to HCT/P products regulated as medical devices.	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)	Required	Type: Boolean	Yes/No	NO	
<b>Latex Information</b>								
<b>Device required to be labeled as containing natural rubber latex or dry natural rubber (21 CFR 801.437)</b>	Indicates that the device or packaging contains natural rubber that contacts humans as described under 21 CFR 801.437. Choosing 'Yes' indicates that the device label or packaging contains one of the following	Choose Yes/No from the drop down list.	None (NO edit, add, or delete are allowed)	Required	Type: Boolean	Yes/No	YES	Public

Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
	statements: (1) "Caution: This Product Contains Natural Rubber Latex Which May Cause Allergic Reactions", (2) This Product Contains Dry Natural Rubber", (3) Caution: The Packaging of This Product Contains Natural Rubber Latex Which May Cause Allergic Reactions" or (4) "The Packaging of This Product Contains Dry Natural Rubber".							
Device labeled as "Not made with natural rubber latex"	Indicates that natural rubber latex was not used as materials in the manufacture of the medical product and container and the device labeling contains this information. Only applicable to devices not subject to the requirements under 21 CFR 801.437. Not all medical products that are NOT made with natural rubber latex will be marked.	Select checkbox if appropriate.  Only applicable if the response to "Device required to be labeled as containing natural rubber latex or dry natural rubber" is "No".  Optional element for labelers who include a statement of 'latex-free' on their label or in their labeling. FDA finds these statements: 'latex-free' and 'does not contain latex', to be not scientifically supportable and	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)	Optional  If no data is provided, "No" is stored	Type: Boolean	NA	NO	Public

Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
		strongly recommends they not be used in medical product labeling. Instead FDA recommends the use of the statement 'Not made with natural rubber latex.' It is not assumed that all devices NOT made with natural rubber latex are marked; therefore this is an optional element for the labelers who choose to make a statement in the labeling.						
<b>Prescription Status</b>								
<b>Prescription Use (Rx)</b>	Indicates that the device requires a prescription to use.	Select checkbox if appropriate. Can select both Rx and OTC for one DI record.	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)	Optional  If no data is provided, "No" is stored	Type: Boolean	NA	NO	Public
<b>Over the Counter (OTC)</b>	Indicates that the device does not require a prescription to use and can be purchased over the counter (OTC).	Select checkbox if appropriate. Can select both Rx and OTC for one DI record.	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)	Optional  If no data is provided, "No" is stored	Type: Boolean	NA	NO	Public
<b>MRI Safety Status</b>								

Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
<p>Is the device labeled for MRI Safety?</p> <p>Removed this attribute as of 5/7/2014</p>	<p>Indicates that sufficient testing has been conducted to characterize the behavior of the device in the MR environment. See ASTM F2503-13.</p>	<p>Check-box if appropriate.</p>	<p>Can Add (Addition of new data is allowed) check to checkbox after Grace Period, but cannot Delete (Deletion of entered data is allowed) a check from the checkbox.</p>	<p>0..1</p>	<p>Boolean</p>	<p>,</p>	<p>NO</p>	<p>Public</p>
<p>MRI Safety Status—What MRI safety information does the labeling contain?</p>	<p>Indicates the MRI Safety Information, if any, that is present in the device labeling. Please see the ASTM F2503-13 standard for more information.</p>	<p>Choose a value from the drop down LOV.</p> <p>The final rule does not require MRI-compatibility testing; it only requires submission of information regarding MRI-compatibility that the labeler already possesses.</p>	<p>Edit (Editing of entered data is allowed)*</p> <p>*ONLY if changing from 'Labeling does not contain...' to other MR status (Safe, Unsafe, ConditionA (data element is not able to be changed directly; most are 'auto-populated' fields whose information depends on another data element)). Otherwise, NO changes are allowed.</p>	<p>Required</p>	<p>NA</p>	<p>MR Safe, MR Unsafe, MR Conditional, Labeling does not contain MRI Safety information</p>	<p>NO</p>	<p>Public</p>
<p>Clinically Relevant Size</p>								

Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
<b>Size Type</b>	Dimension type for the clinically relevant measurement of the medical device.	<p>Choose a value from the drop down LOV.</p> <p>If the desired Size Type is not in the current list, select 'Size Text, specify' and the data element 'Size Type Text' will appear (see below). It is expected that the 'Size Text, specify' will only be available for a limited time. Use this option to help us build a list of values that are appropriate for your device type. GUDID reserves the right to review all suggestions before adding values to the Size Type LOV.</p> <p>More than one Size Value per Type and more than one Size Type may be added to each DI record.</p>	Add (Addition of new data is allowed)	<p>Conditionally Required*</p> <p>*If device is available in more than one size</p>	NA	<p>Circumference; Depth; Device Size Text, specify; Catheter Gauge ; Outer Diameter; Height; Length; Lumen/Inner Diameter; Needle Gauge; Total Volume; Width; Weight; Pressure; Pore Size; Area/Surface Area; Angle</p>	NO	Public
<b>Size Value</b>	Numeric value for the clinically relevant size measurement of the medical device.	<p>Enter numeric value for size. Decimals are accepted; fractions are not accepted. Each Size Value should be entered separately. GUDID is not accepting Size</p>	Add (Addition of new data is allowed)	<p>Conditionally Required*</p> <p>*Required if device is available in more than one size</p>	<p>Type: Num.</p> <p>Length: 40</p>	NA	NO	Public

Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
		Value as a range at this time.						
<b>Size Unit of Measure</b>	<p>"The unit of measure associated with each clinically relevant size.</p> <p>SPL Text: "The unit of measure associated with each clinically relevant size. The unit of measure must conform to UCUM standards."</p>	Choose a value from the drop down.	Add (Addition of new data is allowed)	<p>Conditionally Required*</p> <p>*Required if device is available in more than one size</p>	NA	<p>For length: Centimeter; Decimeter; Feet; Femtometer; Inch; Kilometer; Meter; Micrometer; Millimeter; Nanometer; Picometer; Yard;</p> <p>For area: Square centimeter; Square foot; Square inch; Square meter; Square millimeter;</p> <p>For weight: Gram; Kilogram; Microgram; Milligram; Metric Ton; Pound; Ton</p> <p>For total volume: Centiliter; Cubic Inch; Cup; Deciliter; Femtoliter; Fluid Ounce; Gallon; Kiloliter; Liter; Microliter; Milliliter; Nanoliter; Picoliter; Pint; Quart</p> <p>For gauge: French; Gauge</p> <p>For angle: Degree</p> <p>For pressure: Pound per Square Inch; millibar; KiloPascal; Microgram per Total Volume;</p>	NO	Public

Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
						Milligram per Total Volume; Units per Liter; Hertz;		
<b>Size Type Text</b>  <b>SPL Name: "Size Text"</b>	Additional undefined device size not represented in the GUDID Size Type LOV.	Enter Size Type, Size Unit and Unit of Measure for each entry.	Add (Addition of new data is allowed)	Conditionally Required*  *Required if 'Size Text, specify' is selected above	Type: Alphanum.  Length: 200	NA	NO	Public
<b>Storage and Handling</b>								
<b>Storage and Handling Type</b>	"Indicates storage and handling requirements that are required for the device including temperature, humidity, and atmospheric pressure.  <b>SPL Definition:</b> "Indicates storage requirements are required for the device, including: temperature, humidity, etc."	Choose a value from the drop down LOV.  Conditions of the Storage and Handling Type are measured below as a range, with a Low Value and a High Value. More than one Storage and Handling Type can be added per device record.	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)	Optional	NA	Handling Environment Atmospheric Pressure; Handling Environment Humidity; Handling Environment Temperature; Special Storage Conditions; Storage Environment Atmospheric Pressure; Storage Environment Humidity; Storage Environment Temperature	NO	Public



Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
<b>Low Value</b>  <b>SPL Name:</b> <b>"Storage and Handling Low Value"</b>	"Indicates the low value for storage and handling requirements.  <b>SPL Definition:</b> "Indicates the low value for storage requirements, such as temperature, humidity, etc"	Must enter a Low Value and/or High Value if entering a Storage and Handling Type	Can edit, add, or delete after Grace Period.	00..* A Low Value and/or a High Value is required if Storage and Handling is provided.  <b>SPL Text:</b> "0..1 Conditionally Required* *One value (Low or High) is required if Storage and Handling Type is added to the device record."	Numeric, 6	N/A	NO	Public
<b>High Value</b>  <b>SPL Name:</b> <b>"Storage and Handling High Value"</b>	"Indicates the high value for storage and handling requirements.  <b>SPL Definition:</b> "Indicates the high value for storage requirements, such as temperature, humidity, etc"	<b>Enter a number for High Value.</b>  Must enter at least one value, Low or High but can enter both Low Value and High Value, if needed.  <b>Type:</b> Numeric; <b>Limit:</b> 6 characters	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)	Conditionally Required*  *One value (Low or High) is required if Storage and Handling Type is added to the device record	<b>Type:</b> Num.  <b>Length:</b> 6	NA	NO	Public
<b>Unit of Measure</b>  <b>SPL Name:</b> <b>"Storage and Handling Unit of Measure"</b>	The unit of measure associated with the storage and handling conditions.  <b>SPL Text:</b> "The unit of measure associated with the storage and	Choose a value from the drop down LOV.	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)	Conditionally Required*  *Required if Storage and Handling Type is added to the device record	NA	Degrees Celsius; Degrees Fahrenheit; Degrees Kelvin; Kilo Pascal; Percent (%)	NO	Public

Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
	handling conditions. "The unit of measure associated with the storage and handling conditions. The unit of measure associated with the storage and handling conditions."					Relative Humidity		
<b>Special Storage Conditions</b>	"Indicates any special storage requirements for the device.  SPL Text: "Indicates any special storage requirements for the product."	Enter any other storage conditions. For devices kept at room temperature, or other standard conditions, input that information here.	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)	Conditionally Required*  *Required if 'Special Storage Conditions' is selected above	Type: Alphanumeric.  Length: 200	NA	NO	Public
<b>Sterilization Method</b>								
<b>Device Packaged as Sterile</b>	Indicates the medical device is free from viable microorganisms. See ISO/TS 11139.	Choose Yes/No from the drop down list.  The two Sterilization Method questions are independent of each other; this element is designed to capture information about the device as it enters Commercial Distribution. These data elements are not designed to capture sterilization procedures executed by the	None (NO edit, add, or delete are allowed)	Required	Type: Boolean	Yes/No	YES	Public

Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
		manufacturer or labeler.						
<b>Requires Sterilization Prior to Use</b>	Indicates that the device requires sterilization prior to use.	Choose Yes/No from the drop down list.  The two Sterilization Method questions are independent of each other; this element is designed to capture information about the device before it can safely encounter a patient, regardless of whether the device is single use or reused after reprocessing. These data elements are not designed to capture sterilization procedures executed by the manufacturer or labeler. If answered 'Yes', at least one Sterilization Method (below) must be selected.	None (NO edit, add, or delete are allowed)	Required	Type: Boolean	Yes/No	YES	Public
<b>Sterilization Method</b>	Indicates the method(s) of sterilization that can be used for this device.	Choose a value from the drop down LOV.  Only applicable if the answer to 'Requires Sterilization Prior to Use' is 'Yes'; otherwise, the LOV	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)	Conditionally Required*  *if 'Requires Sterilization Prior to Use' is marked 'Yes'	NA	Chlorine Dioxide; Dry Heat; Ethylene Oxide; High Intensity Light or Pulse Light; Hydrogen Peroxide;	NO	Public



Data Element	Description	Data Entry Notes	Edit (Editing of entered data is allowed) Rules after Grace Period	Required?	Data Type & Length	Entry List of Values (LOV)	New DI Trigger?	Public/Private Status
		will remain inactive.  The Entry LOVs represent the sterilization methods recognized by the CDRH Infection Control Branch. Methods selected should be only those approved for each device by the CDRH Office of Device Evaluation.				Microwave Radiation; Moist Heat or Steam; Ozone; Peracetic Acid; Radiation; Sound Waves; Ultraviolet Light		

## 4. **GS1 GDSN to FDA GUDID Mapping**

Population of the FDA GUDID through the use of a GS1 GDSN message and a GDSN Certified Data Pool as a Third Party requires an understanding of the GDSN and its attributes. While many of the FDA GUDID attributes can be mapped one to one with a GS1 GDSN equivalent, there are others that do not map (and are logically populated) or map via more than one GDSN attribute.

The first table below provides a mapping between the FDA GUDID attribute list and the corresponding GS1 GDSN Attribute(s). The attributes listed in the table use the name assigned in the GDSN standards. Each user of this document should consult with their GDSN Certified Data Pool for the exact naming convention and message formatting applicable to the contract between the user and the Data Pool.

The second table below provides a mapping between the FDA GUDID code values and the corresponding GS1 GDSN code values. The values listed in the table use the name assigned in the GDSN standards. Each user of this document should consult with their GDSN Certified Data Pool for the exact naming convention and message formatting applicable to the contract between the user and the Data Pool.

FDA GUDID Data Element	GS1 GDSN Attribute Name	GDSN Data Type	GDSN Definition	GDSN Notes
<b>Device Information</b>				
<b>Device Identifier (DI) Information</b>				
Issuing Agency	Data Pool to default on outbound message			LOGICAL POPULATION- On the outbound GUDID Message by the Data Pool. Will use the value "GS1" in all GDSN instances.
Primary DI Number	globalTradeItemNumber	Numeric (14 Characters)	EAN.UCC numbering structures will be used for the identification of trade items. All of them will be considered as 14-digit Global Trade Item Number (GTIN). Must be present to enable data to be presented to trade item catalogue. Must be submitted by the owner of the data (who may be the original manufacturer, the importer, the broker or the agent of the original manufacturer). This field is mandatory within the Global Data Synchronization work process.	This GTIN should be the lowest level for the hierarchy.
Device Count	netContent +UoM	Numeric + Code List	The amount of the trade item contained by a package, usually as claimed on the label. For example, Water 750ml - net content = "750 MLT" ; 20 count pack of diapers, net content = "20 ea.". In case of multi-pack, indicates the net content of the total trade item. For fixed value trade items use the value claimed on the package, to avoid variable fill rate issue that arises with some trade item which are sold by volume or weight, and whose actual content may vary slightly from batch to batch. In case of variable quantity trade items, indicates the average quantity.	
Unit of Use DI Number	fDAUnitOfUseGTIN	GTIN	GTIN of a unit of use, as defined by the FDA. This is a lower level unit, which is contained in the Trade Item.	AVP- fDAUnitOfUseGTIN
Labeler DUNS Number	additionalPartyIdentificationType	Code List	Identification of a party by use of a code other than the Global Location Number.	This pair of attributes will be provided as additional party identification for the Brand Owner GLN

FDA GUDID Data Element	GS1 GDSN Attribute Name	GDSN Data Type	GDSN Definition	GDSN Notes
	additionalPartyIdentificationValue	Text	A party identifier that is in addition to the GLN.	
Company Name				FDA will populate based on the DUNS and D&B
Company Physical Address				FDA will populate based on the DUNS and D&B
Brand Name	brandName	Text (1 to 35 characters)	The recognisable name used by a brand owner to uniquely identify a line of trade item or services. This is recognizable by the consumer.	
Version or Model Number	additionalTradeItemIdentificationType	Code List	Type of the identification system that is being used as an alternative to the Global Trade Item Number.	Use code value of MODEL_NUMBER
	additionalTradeItemIdentificationValue	Text	Alternative means to the Global Trade Item Number to identify a trade item.	
Catalog Number	additionalTradeItemIdentificationType	Code List	Type of the identification system that is being used as an alternative to the Global Trade Item Number.	Use code value of SUPPLIER_ASSIGNED
	additionalTradeItemIdentificationValue	Text	Alternative means to the Global Trade Item Number to identify a trade item.	
Device Description (max 2000 characters)	additionalTradeItemDescription	Text (1 to 350 characters)	Additional variants necessary to communicate to the industry to help define the product. Multiple variants can be established for each GTIN. This is a repeatable field, e.g. Style, Colour, and Fragrance. The schema uses common library component as shown in the GDD Max Size field. For the business requirements for item, please use the specific definition of this data type and field, 1-350.	CONCATENATION-tradeItemDescription and additionalTradeItemDescription
	tradeItemDescription	Text (1 to 178 characters)	An understandable and useable description of a trade item using brand and other descriptors. This attribute is filled with as little abbreviation as possible while keeping to a reasonable length. Free form text field, this data element is repeatable	CONCATENATION-tradeItemDescription and additionalTradeItemDescription

FDA GUDID Data Element	GS1 GDSN Attribute Name	GDSN Data Type	GDSN Definition	GDSN Notes
<b>Commercial Distribution</b>				
DI Record Publish Date (mm/dd/yyyy)	uDIDPublishDate	Date (CCYY-MM-DDTHH:MM:SS)	The date upon which the Trade Item can be published by the Unique Device Identifier Database (UDID) in their public facing systems. Until this date, the product information may reside in the UDID, but will not be visible to the public. This data is not changeable and is relationship dependent/specific.	AVP- fDAGUDIDPublishDate
Commercial Distribution End Date (mm/dd/yyyy)	lastShipDate	Date Time (CCYY-MM-DDTHH:MM:SS)	Indicates the latest date that the trade item can be shipped. This is independent of any specific ship-from location.	
Commercial Distribution Status				FDA will populate based on the publication date (effectiveDate) and the lastShipDate.
<b>Alternative or Additional Identifiers</b>				
<b>Direct Marking (DM)</b>				
Device Subject to Direct Marking (DM), but Exempt	isTradeItemExemptFromDirectPartMarking	Boolean	Indicator signifying the trade item is exempt from direct identification marking according to regulation or regulatory filings within the target market.	AVP- isTradeItemExemptFromDirectPartMarking
DM DI Different from Primary DI	Data Pool to default on outbound message	Boolean		LOGICAL POPULATION- (Logical BOOLEAN value of TRUE from the population of a value of DIRECT_PART_MARKING in additionalTradeItemIdentification)
DM DI Number	directPartMarking	Text	This is a number or marking placed directly on the medical device.	AVP- directPartMarking
<b>Secondary DI</b>				



FDA GUDID Data Element	GS1 GDSN Attribute Name	GDSN Data Type	GDSN Definition	GDSN Notes
<a href="#">Secondary DI Issuing Agency</a>	additionalTradeItemIdentificationType	Code List	Type of the identification system that is being used as an alternative to the Global Trade Item Number.	Use code of HIBCC, or ICCBBA
Secondary DI Number	additionalTradeItemIdentificationValue	Code List	Alternative means to the Global Trade Item Number to identify a trade item.	
<b>Package DI</b> Can add Package Configuration after Grace Period, but cannot delete or edit Package Configurations entered prior to the end of the Grace Period.				
Package DI Number	globalTradeItemNumber (use hierarchy to obtain parent-child information)	Numeric (14 Characters)	EAN.UCC numbering structures will be used for the identification of trade items. All of them will be considered as 14-digit Global Trade Item Number (GTIN). Must be present to enable data to be presented to trade item catalogue. Must be submitted by the owner of the data (who may be the original manufacturer, the importer, the broker or the agent of the original manufacturer). This field is mandatory within the Global Data Synchronization work process.	FDA GUDID contains the lowest level of the GDSN hierarchy as its primary. Higher levels of packaging are only referenced as package levels. See additional guidance below for more details.
Quantity per Package	totalQuantityOfNextLowerLevelTradeItem	Numeric	This represents the Total quantity of next lower level trade items that this trade item contains.	
Contains DI Package	childGTIN	Numeric (14 Characters)	A particular Global trade item Number, a numerical value used to uniquely identify a trade item. A trade item is any trade item (trade item or service) upon which there is a need to retrieve pre-defined information and that may be planned, priced, ordered, delivered and or invoiced at any point in any supply chain. In this context, the GTIN for the current item which is a child item of another item.	
Package Type	packagingTypeCode	Text (1-3 characters)	The code identifying the type of package used as a container of the trade item.	
	packagingTypeDescription	Text (1-70 characters)	System generated text description of the type of packaging used for the trade item.	LOGICAL POPULATION- (Logical Population by Data Pools based on the Packaging Type Code value populated.) Only the description is provided to the GUDID

FDA GUDID Data Element	GS1 GDSN Attribute Name	GDSN Data Type	GDSN Definition	GDSN Notes
Package Discontinue Date	discontinuedDate	DateTime	Communicate the date on which the trade item is no longer to be manufactured. Allows the reuse of the GTIN after 48 months with the explicit exception of Apparel, being 30 months and the implicit exception for specialty products (e.g., steel beams).	At the package DI level
Package Status				FDA will populate based on the publication date (effectiveDate) and the lastShipDate.
<b>Support Customer Contact</b>				
	contactType	Code List	The general category of the contact party for a trade item for example Purchasing.	Value populated for the contact information is CUSTOMER_SUPPORT
<b>Support Customer Contact Phone</b>	communicationChannelCode	Code List	Means used to communicate with another party.	Value populated for the support contact phone number is TELEPHONE
	communicationNumber	Text (1-70 characters)	Number assigned to a specific means of communication.	
<b>Support Customer Contact Email</b>	communicationChannelCode	Code List	Means used to communicate with another party.	Value populated for the support contact email is EMAIL
	communicationNumber	Text (1-70 characters)	Number assigned to a specific means of communication.	
<b>Device Status</b>				
Human Cell, Tissue or Cellular or Tissue-Based Product (HCT/P)	doesTradeItemContainHumanTissue	Boolean	The trade item has, as a component or ingredient, human tissue. The amount of tissue is not limited to a certain amount, any amount will cause a flag of TRUE.	AVP-doesTradeItemContainHumanTissue

FDA GUDID Data Element	GS1 GDSN Attribute Name	GDSN Data Type	GDSN Definition	GDSN Notes
Kit	groupedProduct	Code List	Code representing if the trade item is considered by the manufacturer to be more than a single item, such as a kit, combination item.	AVP- groupedProduct (KIT)
				AVP- groupedProduct (KIT_AND_COMBINATION)
Combination Product				AVP- groupedProduct (COMBINATION)
<b>Premarket</b>				
Device Exempt from Premarket Submission	exemptFromFDAPreMarketAuthorization	Boolean	Device is exempt from FDA Premarket regulations. Premarket approval (PMA) is the FDA process of scientific and regulatory review to evaluate the safety and effectiveness of Class III medical devices. Class III devices are those that support or sustain human life, are of substantial importance in preventing impairment of human health, or which present a potential, unreasonable risk of illness or injury. Due to the level of risk associated with Class III devices, FDA has determined that general and special controls alone are insufficient to assure the safety and effectiveness of class III devices. Therefore, these devices require a premarket approval (PMA) application under section 515 of the FD&C Act in order to obtain marketing clearance. Please note that some Class III preamendment devices may require a Class III 510(k). See "Historical Background2" for additional information.	AVP- exemptFromFDAPreMarketAuthorization External Code managed by FDA.
FDA Premarket Submission Number	additionalClassificationCategoryAgency	Code List	Text name of the additional external classification agency whose schema is being provided in addition to the Global EAN.UCC schema. Required if additional classification schema fields	<b>Use code of 58</b> <b>Populate with the FDA Premarket Submission Number. If there is a Supplement Number, place a colon (":") after the Premarket Submission Number then add the Submission Number.</b>

FDA GUDID Data Element	GS1 GDSN Attribute Name	GDSN Data Type	GDSN Definition	GDSN Notes
			are populated.	Repeat these attributes and process for all applicable FDA Premarket Submission Numbers and Supplement Numbers.
	additionalClassificationCategoryCode	Text (1-15 characters)	Category code based on alternate classification schema chosen in addition to EAN/UCC classification schema.	
Supplement Number	See FDA Premarket Submission Number			See FDA Premarket Submission Number
<b>FDA Product Code</b>				
Product Code	additionalClassificationCategoryAgency	Code List	Text name of the additional external classification agency whose schema is being provided in addition to the Global EAN.UCC schema. Required if additional classification schema fields are populated.	Use code 43- US FDA Product Code Classification Database: The Product Classification Database contains medical device names and associated information developed by the Center for Devices and Radiological Health (CDRH) in support of its mission. This database contains device names and their associated product codes. The name and product code identify the generic category of a device for FDA. The Product Code assigned to a device is based upon the medical device product classification designated under 21 CFR Parts 862-892.
	additionalClassificationCategoryCode	Text (1-15 characters)	Category code based on alternate classification schema chosen in addition to EAN/UCC classification schema.	Code value managed by FDA.
Product Code Name				FDA will populate based on the FDA Product Code
<b>FDA Listing</b>				
FDA Listing Number	additionalTradeItemIdentificationType	Code List	Type of the identification system that is being used as an alternative to the Global Trade Item Number.	AVP- fDAMedicalDeviceListing

FDA GUDID Data Element	GS1 GDSN Attribute Name	GDSN Data Type	GDSN Definition	GDSN Notes
	additionalTradeItemIdentificationValue	Code List	Alternative means to the Global Trade Item Number to identify a trade item.	
<b>GMDN</b>				
Code  SPL Name- GMDN Preferred Term Code	additionalClassificationAgency	Code List	Section 510(k) of the Food, Drug and Cosmetic Act requires device manufacturers who must register, to notify FDA of their intent to market a medical device at least 90 days in advance. This is known as Premarket Notification - also called PMN or 510(k). This allows FDA to determine whether the device is equivalent to a device already placed into one of the three classification categories. Specifically, medical device manufacturers are required to submit a premarket notification if they intend to introduce a device into commercial distribution for the first time or reintroduce a device that will be significantly changed or modified to the extent that its safety or effectiveness could be affected. Such change or modification could relate to the design, material, chemical composition, energy source, manufacturing process, or intended use.	Use code 35
	additionalClassificationCode	Text (1-15 characters)	Category code based on alternate classification schema chosen in addition to EAN/UCC classification schema.	Code value managed by GMDN. Only the GMDN Code is provided to the GUDID
Name	additionalClassificationCategoryDescription	Text (1-70 characters)	In the additional classification system, the description of the category.	FDA will populate based on the FDA Product Code. Can be provided via GDSN for supply chain purposes, but will not be populated to the GUDID from GDSN.

FDA GUDID Data Element	GS1 GDSN Attribute Name	GDSN Data Type	GDSN Definition	GDSN Notes
Definition				FDA will populate based on the FDA Product Code
SPL Name- FDA Preferred Term Code	additionalClassificationCategoryCode	Text (1-15 characters)	Category code based on alternate classification schema chosen in addition to EAN/UCC classification schema.	Code value managed by GMDN/FDA. Only either the GMDN or FDA Code is provided to the GUDID, the FDA will derive the actual term from a mapping to the GMDN or FDA Preferred term listing.
<b>Device Characteristics</b>				
For Single-Use	manufacturerDeclaredReusabilityType	Code List	Determines if the product is intended for single or multiple uses; including the number of validated cycles and the number of times a product can be used according to the manufacturer specifications. It is suggested that medical providers consult the device manufacturer's Instruction For Use (IFU) for full reusability instructions.	LOGICAL POPULATION- (Logical BOOLEAN value of TRUE from the population of a value of SINGLE_USE in manufacturerDeclaredReusabilityType, all other values equate to a FALSE value)
<b>Production Identifier(s) on Label</b>				
Lot or Batch Number	hasBatchNumber	Boolean	Indication whether the base trade item is batch or lot number requested by law, not batch or lot number requested by law but batch or lot number allocated, or not batch or lot number allocated. A batch or lot number is a manufacturer assigned code used to identify a trade item's trade item on batch or lot. Differs from Serial Number which is a manufacturer assigned code during the trade item on cycle to identify a unique trade item.	

FDA GUDID Data Element	GS1 GDSN Attribute Name	GDSN Data Type	GDSN Definition	GDSN Notes
Manufacturing Date	isPackageMarkedWithManufactureDate	Boolean	Is the package marked with the date upon which the trade item was manufactured.	AVP- isPackageMarkedWithManufactureDate
Serial Number	serialNumberLocationCode	Text (1-35 characters)	The location on the item or packaging of a serial number. A serial number is a code, numeric or alphanumeric, assigned to an individual instance of an entity for its lifetime for example a Microscope model AC-2 with serial number 1234568 and microscope model AC-2 with serial number 1234569.	LOGICAL POPULATION- (Logical BOOLEAN value of TRUE from the population of any value except NOT_MARKED in serialNumberLocationCode)
Expiration Date	packagingMarkedExpirationDateType	Code List	Indicates the type of expiration date marked on the packaging.	LOGICAL POPULATION- (Logical BOOLEAN value of TRUE from the population of either values of BEST_BEFORE_DATE or EXPIRY_DATE in packagingMarkedExpirationDateType (changing to tradeItemDateOnPackagingType (coming in GDSN Major Release 3.x in 2016) other values or when no value is provided would equate to a value of FALSE)
Donation Identification Number	donationIdentificationNumberMarked	Boolean	Indicates the device is managed by a Donation Identification Number. This number can be found on the device label or packaging. The Donation Identification Number is applicable to devices that are also regulated as HCT/Ps and is a number that is assigned to each donation.	AVP- donationIdentificationNumberMarked
<b>Latex Information</b>				
Device required to be labeled as containing natural rubber latex or dry natural rubber (21 CFR 801.437)	doesTradeItemContainLatex	Non-Binary Code List	An indication that a trade item is made from or contains latex which refers generically to a stable dispersion (emulsion) of polymer microparticles in an aqueous medium.	This definition is currently listed on the Global Data Dictionary, but will be changed in a future GDSN release to the definition and wording at this link. Please use this new wording when populating the attribute.
Device labeled as "Not made with natural rubber latex"	packageMarksFreeFrom	Code List	Indication of the food ingredients that the package is marked free from.	Use value of FREE_FROM_LATEX
<b>Prescription Status</b>				

FDA GUDID Data Element	GS1 GDSN Attribute Name	GDSN Data Type	GDSN Definition	GDSN Notes
Prescription Use (Rx)	ConsumerSalesCondition	Text (1-35 characters)	A code depicting restrictions imposed on the Trade Item regarding how it can be sold to the consumer for example Prescription Required.	Use value of PRESCRIPTION_REQUIRED
Over the Counter (OTC)				Use value of OTC
<b>MRI Safety Status</b>				
<p>Is the device labeled for MRI Safety?</p> <p>removed this attribute as of 4/16/2014</p>	Data Pool to default on outbound message	:	:	LOGICAL POPULATION- (Logical BOOLEAN value of TRUE from the population of any value other than UNKNOWN in mRICompatibility)
<p><u>MRI Safety Status-What MRI safety information does the labeling contain?</u></p>	mRICompatibility	Code List	This is an identification of the compatibility of a trade item for use in the presence of a Magnetic Resonance Imaging (MRI) system.	
<b>Clinically Relevant Size</b>				
Size Type	clinicalSizeType	Code List	The qualifier to denote the dimensional size which is clinically relevant for the use of the trade item by the clinical user. For example "needle gauge" for a 16 gauge needle, or "volume" for a 200 cc syringe.	AVP- clinicalSizeType
Size Value	clinicalSizeValue + UoM	Numeric + Code List	The value to denote the dimensional size, which is clinically relevant for the use of the trade item by the clinical user. For example 16 gauge for a needle, or 200 cc for a syringe. Carries a UoM from the Recommendation 20 code list.	AVP- clinicalSizeValue and clinicalSizeValueUoM
Size Unit of Measure				
<p>Size Type Text</p> <p>SPL Name: "Size Text"</p>	clinicalSizeText	Text (1 to 200 characters)	When the clinicalSizeType is coded as "other", this is the text used to denote the dimensional size, which is clinically relevant for the use of the trade item by the clinical user.	AVP- clinicalSizeText
<b>Storage and Handling</b>				



FDA GUDID Data Element	GS1 GDSN Attribute Name	GDSN Data Type	GDSN Definition	GDSN Notes
Storage and Handling Type	storageEnvironmentAtmosphericPressureMaximum + UoM	Numeric + Code List	The maximum atmospheric pressure in which the item should be stored to remain usable. This value is the value above which the trade item should not be subjected.	AVP- storageEnvironmentAtmosphericPressureMaximum  AVP- storageEnvironmentAtmosphericPressureMinimum
	storageEnvironmentAtmosphericPressureMinimum + UoM	Numeric + Code List	The minimum atmospheric pressure in which the item should be stored to remain usable. This value is the value below which the trade item should not be subjected.	GUDID Code for Storage Type- Storage Environment Atmospheric Pressure
High Value	storageEnvironmentAtmosphericPressureMaximum + UoM	Numeric + Code List	The maximum atmospheric pressure in which the item should be stored to remain usable. This value is the value above which the trade item should not be subjected.	AVP- storageEnvironmentAtmosphericPressureMaximum  High Value for GUDID Code for Storage Type- Storage Environment Atmospheric Pressure
Unit of Measure				
Low Value	storageEnvironmentAtmosphericPressureMinimum + UoM	Numeric + Code List	The minimum atmospheric pressure in which the item should be stored to remain usable. This value is the value below which the trade item should not be subjected.	AVP- storageEnvironmentAtmosphericPressureMinimum  Low Value for GUDID Code for Storage Type- Storage Environment Atmospheric Pressure
Unit of Measure				
Storage and Handling Type	storageHandlingHumidityMaximum + UoM	Numeric + Code List	The maximum humidity in percentages that the goods should be stored in.	GUDID Code for Storage Type- Storage environment humidity
	storageHandlingHumidityMinimum + UoM	Numeric + Code List	The minimum humidity in percentages that the goods should be stored in.	
High Value	storageHandlingHumidityMaximum + UoM	Numeric + Code List	The maximum humidity in percentages that the goods should be stored in.	High Value for GUDID Code for Storage Type- Storage environment humidity
Unit of Measure				
Low Value	storageHandlingHumidityMinimum + UoM	Numeric + Code List	The minimum humidity in percentages that the goods should be stored in.	Low Value GUDID Code for Storage Type- Storage environment humidity
Unit of Measure				

FDA GUDID Data Element	GS1 GDSN Attribute Name	GDSN Data Type	GDSN Definition	GDSN Notes
Storage and Handling Type	storageHandlingTemperatureMaximum + UoM	Numeric + Code List	The maximum temperature at which the trade item can be stored. This uses a measurement consisting of a unit of measure and a value.	GUDID Code for Storage Type- Storage environment temperature
	storageHandlingTemperatureMinimum + UoM	Numeric + Code List	The minimum temperature at which the trade item can be stored. This uses a measurement consisting of a unit of measure and a value.	
High Value SPL Name: "Storage and Handling High Value"	storageHandlingTemperatureMaximum + UoM	Numeric + Code List	The maximum temperature at which the trade item can be stored. This uses a measurement consisting of a unit of measure and a value.	High value for GUDID Code for Storage Type- Storage environment temperature
Unit of Measure SPL Name: "Storage and Handling Unit of Measure"				
Low Value SPL Name: "Storage and Handling Low Value"	storageHandlingTemperatureMinimum + UoM	Numeric + Code List	The minimum temperature at which the trade item can be stored. This uses a measurement consisting of a unit of measure and a value.	Low value for GUDID Code for Storage Type- Storage environment temperature
Unit of Measure SPL Name: "Storage and Handling Unit of Measure"				
Storage and Handling Type	transportationEnvironmentAtmospheric PressureMaximum + UoM	Numeric + Code List	The maximum atmospheric pressure in which the item should be transported to remain usable. This value is the value above which the trade item should not be subjected.	AVP- transportationEnvironmentAtmosphericP ressureMaximum
	transportationEnvironmentAtmospheric PressureMinimum + UoM	Numeric + Code List	The minimum atmospheric pressure in which the item should be transported to remain usable. This value is the value below which the trade item should not be subjected.	AVP- transportationEnvironmentAtmosphericP ressureMinimum GUDID Code for Storage Type- Handling Environment Atmospheric Pressure
High Value SPL Name: "Storage and Handling High Value"	transportationEnvironmentAtmospheric PressureMaximum + UoM	Numeric + Code List	The maximum atmospheric pressure in which the item should be transported to remain usable. This value is the value above which the trade item should not be subjected.	AVP- transportationEnvironmentAtmosphericP ressureMaximum
Unit of Measure SPL Name: "Storage and Handling Unit of Measure"				High Value for GUDID Code for Storage Type- Handling Environment Atmospheric Pressure

FDA GUDID Data Element	GS1 GDSN Attribute Name	GDSN Data Type	GDSN Definition	GDSN Notes
Low Value SPL Name: "Storage and Handling Low Value"	transportationEnvironmentAtmosphericPressureMinimum + UoM	Numeric + Code List	The minimum atmospheric pressure in which the item should be transported to remain usable. This value is the value below which the trade item should not be subjected.	AVP-transportationEnvironmentAtmosphericPressureMinimum
Unit of Measure SPL Name: "Storage and Handling Unit of Measure"				Low Value for GUDID Code for Handling Environment Atmospheric Pressure
Storage and Handling Type	transportationHumidityMaximum + UoM	Numeric + Code List	The maximum humidity in percentages in which the trade items should be transported.	AVP-transportationMaximumHumidityMaximum
	transportationHumidityMinimum + UoM	Numeric + Code List	The minimum humidity in percentages in which the trade items should be transported.	AVP-transportationMaximumHumidityMinimum GUDID Code for Storage Type-- Handling environment humidity
High Value SPL Name: "Storage and Handling High Value"	transportationHumidityMaximum + UoM	Numeric + Code List	The maximum humidity in percentages in which the trade items should be transported.	High Value for GUDID Code for Storage Type- Handling environment humidity
Unit of Measure SPL Name: "Storage and Handling Unit of Measure"				
Low Value SPL Name: "Storage and Handling Low Value"	transportationHumidityMinimum + UoM	Numeric + Code List	The minimum humidity in percentages in which the trade items should be transported.	Low value for GUDID Code for Storage Type- Handling environment humidity
Unit of Measure SPL Name: "Storage and Handling Unit of Measure"				
Storage and Handling Type	transportationMaximumTemperature + UoM	Numeric + Code List	The maximum temperature that a trade item can be held at during transport as defined by the manufacturer without affecting product safety or quality.	GUDID Code for Storage Type- Handling environment temperature
	transportationMinimumTemperature + UoM	Numeric + Code List	The minimum temperature that a trade item can be held below during transport as defined by the manufacturer without affecting product safety or quality.	
High Value SPL Name: "Storage and Handling High Value"	transportationMaximumTemperature + UoM	Numeric + Code List	The maximum temperature that a trade item can be held at during transport as defined by the manufacturer without affecting product safety or	High value for GUDID Code for Storage Type- Handling environment temperature

FDA GUDID Data Element	GS1 GDSN Attribute Name	GDSN Data Type	GDSN Definition	GDSN Notes
Unit of Measure <b>SPL Name: "Storage and Handling Unit of Measure"</b>			quality.	
Low Value <b>SPL Name: "Storage and Handling Low Value"</b>	transportationMinimumTemperature + UoM	Numeric + Code List	The minimum temperature that a trade item can be held below during transport as defined by the manufacturer without affecting product safety or quality.	Low value for GUDID Code for Storage Type- Handling environment temperature
Unit of Measure <b>SPL Name: "Storage and Handling Unit of Measure"</b>				
Special Storage Conditions	consumerUsageStorageInstructions	Text (1 to 1000 characters)	Expresses in text the consumer storage and usage instructions of a product which are normally held on the label or accompanying the product. This information may or may not be labelled on the pack. Instructions may refer to a suggested storage temperature, a specific storage requirement or a reference to environment or duration. Examples include: "Refrigerate After Opening", "Consume within 4 days", "Keep Out Of Direct Sunlight", "Store at an Ambient Temperature", "Store in a Clean, Cool, Dry Place", "Store Away From Sunlight, Strong Odours and Chemicals", "Keep in a Clean, Cool, Dry and Odourless Place Away From Direct Sunlight and Freezing Temperatures", "Keep in a Clean, Cool, Dry and Odourless Place Away From Direct Sunlight", "Before opening store at + 5°C+ 30°C", "After Opening Keep Refrigerated (+5°C) and Consume Within 48 hours", "Drink Chilled", "Store in a Cool Dry Place", "Refrigerate After Opening. Can Be Kept in the Fridge For 3 Months".	
<b>Sterilization Method</b>				

FDA GUDID Data Element	GS1 GDSN Attribute Name	GDSN Data Type	GDSN Definition	GDSN Notes
Device Packaged as Sterile	initialManufacturerSterilisation	Code List	Type(s) of sterilisation that may have been performed by the manufacturer if a trade item is sterile when it comes from the manufacturer. Sterilisation refers to any process that effectively kills or eliminates transmissible agents (such as fungi; bacteria; viruses; prions and spore forms etc.) from a surface; equipment; foods; medications; or biological culture medium. Some methods of sterilisation are through the application of heat; radiation; and ethylene.	LOGICAL POPULATION- (Logical BOOLEAN value of TRUE from the population of any value in initialManufacturerSterilisation)
Requires Sterilization Prior to Use	Data Pool to default on outbound message			LOGICAL POPULATION- (Logical BOOLEAN value of TRUE from the population of any value in initialSterilisationPriorToUse)
Sterilization Method	initialSterilisationPriorToUse	Code List	This is an indication of the type(s) of sterilisation that is required to be completed by a healthcare provider prior to initial use of the healthcare trade item. Sterilisation refers to any process that effectively kills or eliminates transmissible agents (such as fungi; bacteria; viruses; prions and spore forms etc.) from a surface; equipment; foods; medications; or biological culture medium. Some methods of sterilisation are through the application of heat; radiation; and ethylene.	

## 5. FDA GUDID mapping to GS1 code values

The list below are FDA GUDID code values mapped to GS1 GDSN Code values. For some of these attributes, there may be additional code values available for use in GDSN not listed. This list focuses on just the values applicable to the GUDID mapping. Where the terming “PENDING” is utilized, it means actual code values have either not been identified by the FDA, or that a code is in process with the Global Standards Management Process (GSMP), but not yet assigned.

FDA GUDID Code- Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
Version or Model Number		Additional Trade Item Identification Type	MODEL_NUMBER		<p>(Current definition)- Additional Vendor identification number, which defines the configuration of the product over and above the Item number.</p> <p>(Definition for GDSN Major Release 3.x in 2016)- The additional Trade Item Identification value populated is an identification number which defines the configuration of the product in addition to the Item number. This is typically printed or otherwise attached to an item. In electronics, this number is typically found around or near a serial number.</p>

FDA GUDID Code- Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
Catalog Number		Additional Trade Item Identification Type	SUPPLIER_ASSIGNED		<p>(Current definition)- The additional Trade Item Identification value populated has been developed and assigned by the party which provides service(s) and/or manufactures or otherwise has possession the goods and consigns or makes them available in trade.</p> <p>(Definition for GDSN Major Release 3.x in 2016)- The additional Trade Item Identification value populated has been developed and assigned by the party which provides service(s) and/or manufactures or otherwise has possession of the goods and consigns or makes them available in trade. This number is a base model or style number assigned to the product and may be the same for several GTINs where they are variations of each other. For example a coffee mug with 3 GTINs one each for the brown mug, the white mug, and the black mug might all be the supplier assigned number of AB123. Use of this value is recommended in the absence of a Model Number or Manufacturer's Part Number.</p>
Contact	Used to provide Contact Information for GUDID	Contact Type	CONSUMER_SUPPORT		The party which provides product support to the end user of a trade item or a service.
Device labeled as "Not made with natural rubber latex"	FALSE	packageMarksFreeFrom	FREE_FROM_EGG		Marks if the product is free from egg.
Device labeled as "Not made with natural rubber latex"	FALSE	packageMarksFreeFrom	FREE_FROM_FISH		The item is physically marked as being free from fish, as approved by the appropriate authority of the target market.
Device labeled as "Not made with natural rubber latex"	FALSE	packageMarksFreeFrom	FREE_FROM_GLUTEN		Marks if the product is free from gluten. This level of containment is frequently determined through regulation for example per EU Regulation (EC) No 41/2009 [of 20 January 2009], this is defined as =< 20 mg/kg).
Device labeled as "Not made with natural rubber latex"	FALSE	packageMarksFreeFrom	FREE_FROM_LACTOSE		Indicates if the amount of lactose is reduced.
Device labeled as "Not made with natural rubber latex"	TRUE	packageMarksFreeFrom	FREE_FROM_LATEX		The item is physically marked being free from Latex (rubber) as approved by the appropriate authority of the

FDA GUDID Code- Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
					target market.
Device labeled as "Not made with natural rubber latex"	FALSE	packageMarksFreeFrom	FREE_FROM_LEGUME_PROTEIN		The item is physically marked as being free from legume protein, as approved by the appropriate authority of the target market.
Device labeled as "Not made with natural rubber latex"	FALSE	packageMarksFreeFrom	FREE_FROM_MILK		The item is physically marked as being free from milk and any of its derivatives, as approved by the appropriate authority of the target market.
Device labeled as "Not made with natural rubber latex"	FALSE	packageMarksFreeFrom	FREE_FROM_MILK_PROTEIN		Free from milk protein.
Device labeled as "Not made with natural rubber latex"	FALSE	packageMarksFreeFrom	FREE_FROM_NATURAL_GLUTEN		The item is physically marked as being naturally free from gluten and not extracted as part of the manufacturing process, as approved by the appropriate authority of the target market.
Device labeled as "Not made with natural rubber latex"	FALSE	packageMarksFreeFrom	FREE_FROM_PEAUTS		Marks if the product is free from peanuts.
Device labeled as "Not made with natural rubber latex"	FALSE	packageMarksFreeFrom	FREE_FROM_PROTEIN		The item is physically marked as being free from protein, as approved by the appropriate authority of the target market.
Device labeled as "Not made with natural rubber latex"	FALSE	packageMarksFreeFrom	FREE_FROM_PVC		The item is physically marked as being free from PVC (Polyvinyl chloride), as approved by the appropriate authority of the target market.
Device labeled as "Not made with natural rubber latex"	FALSE	packageMarksFreeFrom	FREE_FROM_SOYA		Free from soya.
Device labeled as "Not made with natural rubber latex"	FALSE	packageMarksFreeFrom	FREE_FROM_SUGAR		Marks if the product is free from sugar.
Device labeled as "Not made with natural rubber latex"	FALSE	packageMarksFreeFrom	REDUCED_LACTOSE		Indicates if the amount of lactose is reduced.
Device labeled as "Not made with natural rubber latex"	FALSE	packageMarksFreeFrom	REDUCED_PROTEIN		The item is physically marked as containing a low level of protein as approved by the appropriate authority of the target market.
Device labeled as "Not made with natural rubber latex"	FALSE	packageMarksFreeFrom	VERY_LOW_GLUTEN		The item is physically marked as a very low amount of gluten. Very low is frequently determined through regulation for example, per EU Regulation (EC) No 41/2009 [of 20 January 2009], this is defined as containing between 20 and 100 mg/kg).
Device labeled as "Not made with natural rubber latex"	FALSE	packageMarksFreeFrom	WITHOUT_ADDED_SUGAR		The item is physically marked that no sugar has been added when manufacturing the product but it still



FDA GUDID Code- Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
					can contain sugars that are naturally part of the ingredients, as approved by the appropriate authority of the target market.
Device labeled as "Not made with natural rubber latex"	FALSE	packageMarksFreeFrom	WITHOUT_ADDED_SW EETENER		The item is physically marked that no sweetener has been added when manufacturing the product as approved by the appropriate authority of the target market.
Device required to be labeled as containing natural rubber latex or dry natural rubber (21 CFR 801.437)	FALSE	Does Trade Item Contain Latex	FALSE		The Brand Owner labeling does not state the Trade Item contains latex or may state that the Trade Item is free from latex.
Device required to be labeled as containing natural rubber latex or dry natural rubber (21 CFR 801.437)	TRUE	Does Trade Item Contain Latex	TRUE		Brand Owner labeling states the Trade Item contains latex.
Expiration Date	TRUE	Packaging Marked Expiration Date Type	BEST_BEFORE_DATE		Not Applicable
Expiration Date	TRUE	Packaging Marked Expiration Date Type	EXPIRY_DATE		Not Applicable
Expiration Date	Other values or no value populated equates to a value of FALSE	Packaging Marked Expiration Date Type			
<b>GMDN Preferred Term Code</b>	<b>GMDN Preferred Term Code</b>	additionalClassificationAge ncyName	35	GMDN	Global Medical Devices Nomenclature (GMDN)
<b>FDA Preferred Term Code</b>	<b>FDA Preferred Term Code</b>	<b>additionalClassificationAge ncyName</b>	<b>PENDING</b>		
FDA Product Code	FDA Product Code	additionalClassificationAge ncyName	43	FDA Product Code	US FDA Product Code Classification Database: The Product Classification Database contains medical device names and associated information developed by the Center for Devices and Radiological Health (CDRH) in support of its mission. This database contains
FDA Premarket Submission Number	FDA Premarket Submission Number	additionalClassificationAge ncyName	58	FDA Premarket Submission Number	
For GDS Use Only		additionalClassificationAge ncyName	5	UNSPSC	UNSPSC: United Nations Standard Products and Services Code
For GDS Use Only		additionalClassificationAge ncyName	6	UNSPSC- ECCMA	UNSPSC - Electronic Commerce Code Management Association
For Single Use	FALSE	Healthcare Trade Item Reusability	LIMITED_REUSABLE		Manufacturer has indicated that product may be reused but has provided special instructions, limitations or guidelines around the reuse of this trade item.
For Single Use	FALSE	Healthcare Trade Item	REUSABLE		Product can be reused

FDA GUDID Code- Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
		Reusability			
For Single Use	TRUE	Healthcare Trade Item Reusability	REUSABLE_SAME_PATIENT		Product can only be reused for the same patient.
For Single Use	TRUE	Healthcare Trade Item Reusability	SINGLE_USE		Item is not intended to be reused.
Labeler DUNS		Additional Party Identification Type	DUNS		N/A
Labeler DUNS		Additional Party Identification Type	DUNS_PLUS_FOUR		N/A
MRI Safety Status	MR Conditional	mRICompatibility	MRI_CONDITIONAL		Indicates that a healthcare trade item is safe to use under specified conditions in a Magnetic Resonance Imaging (MRI) System
MRI Safety Status	MR Safe	mRICompatibility	MRI_SAFE		Indicates that the healthcare trade item is safe to use within a Magnetic Resonance Imaging (MRI) system.
MRI Safety Status	MR Unsafe	MRCompatibility	MRI_UNSAFE		Indicates that a healthcare trade item is not safe to use in an MRI system.
MRI Safety Status	Labeling does not contain MRI Safety Information	MRCompatibility	UNSPECIFIED		The manufacturer of the Trade Item has not communicated information on the compatibility of this trade item with a Magnetic Resonance Imaging (MRI) System.
Over the Counter (OTC)	Over the Counter (OTC)	Consumer Sales Conditions	OTC		Over the Counter- products that may be sold without a prescription. These products are generally available without restrictions.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	AAA	Pallet, Returnable	Pallet, Returnable
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	AAB	Splash Blend	Splash Blend- Splash blending is the mixing of two gasoline products, of different octane levels, in a tank on the delivery vehicle to produce a third blended grade of motor fuel for resale
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in	Packaging Type Code	AE	Aerosol	Aerosol: A gas-tight, pressure-resistant container with a valve and propellant. When the valve is opened, propellant forces the product from the container in a fine

FDA GUDID Code- Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
	the description field at right should be passed to the FDA GUDID.				or coarse spray pattern or stream. (e.g., a spray can dispensing paint, furniture polish
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	AMM	Ammo Pack	Ammo Pack
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	AMP	Ampoule	Ampoule: A relatively small container made from glass or plastic tubing, the end of which is drawn into a stem and closed by fusion after filling. The bottom may be flat, convex, or drawn out. An ampule is opened by breaking the stem.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	AT	Atomizer	Atomizer: A device for reducing a liquid to a fine spray. (e.g..., medicine, perfume, etc). An atomizer does not rely on a pressurised container for the propellant. Usually air is provided by squeezing a rubber bulb attached to the atomizer.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	ATH	Attachment	Attachment: In containers and shipping devices, a component that can be added to provide additional functionality or security as required by the contents or method of transportation/handling
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	BAG	Bag	Bag: A preformed, flexible container, generally enclosed on all but one side, which forms an opening that may or may not be sealed after filling.
Packaging Type	GDSN utilizes the code value, however	Packaging Type Code	BAL	Bale	Bale

FDA GUDID Code- Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
	GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.				
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	BBL	Barrel	Barrel: A cylindrical packaging whose bottom end is permanently fixed to the body and top end (head) is either removable or non-removable.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	BDG	Banding	Banding: Something that binds, ties, or encircles the package/container to secure and maintain unit integrity
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	BDL	Bundle	Bundle
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	BEM	Beam	Beam
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA	Packaging Type Code	BIC	Bing Chest	Bing Chest

FDA GUDID Code- Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
	GUDID.				
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	BIN	Bin	Bin
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	BLK	Bulk	Bulk
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	BLT	Belting	Belting: As pertains to containers and shipping devices, a method of securing the contents to the conveyance device (or securing components of the shipping device to each other) using one or more bands of flexible material having high-tensile strength and
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	BME	Blister Pack	<b>Blister Pack: A type of packaging in which the item is secured between a preformed (usually transparent plastic) dome or "bubble" and a surface or "carrier." Attachment may be by stapling, heatsealing, gluing, or other means. In other instances, the blister folds over the product in clam-shell fashion to form an enclosing container. Blisters are most usually thermoformed from polyvinyl chloride; however, almost any thermoplastic can be thermoformed into a blister.</b>
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA	Packaging Type Code	BOB	Bobbin	Bobbin

FDA GUDID Code- Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
	GUDID.				
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	BOT	Bottle	Bottle: A container having a round neck of relatively smaller diameter than the body and an opening capable of holding a closure for retention of the contents. Specifically, a narrow-necked container as compared with a jar or wide-mouth container. The c
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	BOX	Box	<b>Box: A non-specific term used to refer to a rigid, three-dimensional container with closed faces that completely enclose its contents and may be made out of any material. Even though some boxes might be reused or become resealed they could also be disposable depending on the product hierarchy.</b>
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	BRC	Bracing	Bracing: Material or devices used to hold articles or sections of loads in position to prevent shifting during transportation
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	BRG	Barge	Barge
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	BSK	Basket or hamper	Basket or hamper: A semi rigid container usually open at the top traditionally used for gathering, shipping and marketing agricultural products.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the	Packaging Type Code	BXI	Box, with inner container	Box, with inner container

FDA GUDID Code- Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
	code. The term in the description field at right should be passed to the FDA GUDID.				
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	BXT	Bucket	Bucket: A container, usually cylindrical, can be equipped with a lid and a handle. (e.g., a pail made of metal, plastic, or other appropriate material).
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	CAB	Cabinet	Cabinet
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	CAG	Cage	Cage: A container enclosed on at least one side by a grating of wires or bars that lets in air and light.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	CAN	Can	Can: A metallic and generally cylindrical container of unspecified size which can be used for items of consumer and institutional sizes.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	CAR	Carrier	Carrier

FDA GUDID Code- Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	CAS	Case	Case: A non-specific term for a container designed to hold, house, and sheath or encase its content while protecting it during distribution, storage and/or exhibition. Cases are mostly intended to store and preserve its contents during the product's entire lifetime.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	CBC	Containers of Bulk Cargo	Containers of Bulk Cargo
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	CBY	Carboy	Carboy
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	CCS	Can Case	Can Case
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	CG	Card	Card: A flat package to which the product is hung or attached for display.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field	Packaging Type Code	CHE	Cheeses	Cheeses



FDA GUDID Code- Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
	at right should be passed to the FDA GUDID.				
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	CHS	Chest	Chest
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	CLD	Car Load, Rail	Car Load, Rail
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	CMS	Clamshell	Clamshell
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	CNA	Household Goods Container, Wood	Household Goods Container, Wood
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	CNB	Container, MAC-ISO, LT. WGT. 8x8x20 Foot Air	Container, MAC-ISO, LT. WGT. 8x8x20 Foot Air
Packaging Type	GDSN utilizes the code value, however GUDID currently	Packaging Type Code	CNC	Container, Navy Cargo Transporter	Container, Navy Cargo Transporter

FDA GUDID Code- Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
	needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.				
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	CND	Container, Commercial Highway Lift	Container, Commercial Highway Lift
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	CNE	Container, Engine	Container, Engine
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	CNF	Container, Multi-walled, Secured to Warehouse Pallet	Container, Multi-walled, Secured to Warehouse Pallet
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	CNT	Container	Container
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	COL	Coil	Coil

FDA GUDID Code- Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	CON	Cones	Cones
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	COR	Core	Core
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	CRD	Cradle	Cradle
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	CRF	Corner Reinforcement	Corner Reinforcement: Usually in boxes or crates, additional material or components attached to adjacent panels to add support or prevent crushing or separation
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	CRT	Crate	<b>Crate: A non-specific term usually referring to a rigid three-dimensional container with semi-closed faces that enclose its contents for shipment or storage. Crates could have an open or closed top and may have internal dividers. Even though some crates might be reused or become resealed they could also be disposable depending on the product hierarchy.</b>
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the	Packaging Type Code	CSK	Cask	Cask

FDA GUDID Code- Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
	code. The term in the description field at right should be passed to the FDA GUDID.				
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	CTN	Carton	Carton: A non-specific term for a re-closable container used mostly for perishable foods (e.g. eggs, fruit).
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	CU	Cup	Cup: A small bowl shaped container for beverages, often with a handle.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	CX2	CONEX	CONEX: A reusable container for shipment of cargo
Packaging Type	GDSN utilizes the code value; however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	CYL	Cylinder	Cylinder: A rigid cylindrical container with straight sides and circular ends of equal size.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	DBK	Dry Bulk	Dry Bulk

FDA GUDID Code- Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	DRK	Double-length Rack	Double-length Rack
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	DRM	Drum	Drum
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	DSK	Double-length Skid	Double-length Skid
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	DTB	Double-length Tote Bin	Double-length Tote Bin
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	DUF	Duffelbag	Duffelbag
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field	Packaging Type Code	EGG	Egg Crating	Egg Crating: In containers and shipping devices, usually describes a type of interior dunnage which allows the contents to be individually segregated, horizontally and vertically, to provide protection

FDA GUDID Code- Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
	at right should be passed to the FDA GUDID.				during transportation and storage
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	ENV	Envelope	<b>Envelope: A predominantly flat container of flexible material having only two faces, and joined at three edges to form an enclosure. The non-joined edge provides a filling opening, which may later be closed by a gummed or adhesive flap, heat seal, tie string, metal clasp, or other methods.</b>
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	EPR	Edge Protection	Edge Protection: A right-angle piece placed over the outermost perimeter edges of a container to distribute pressure and prevent collapse or cutting from banding, strapping, or handling
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	FIR	Firkin	Firkin
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	FLO	Flo-bin	Flo-bin
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	FRM	Frame	Frame
Packaging Type	GDSN utilizes the code value, however GUDID currently	Packaging Type Code	FSK	Flask	Flask

FDA GUDID Code- Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
	needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.				
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	FWR	Forward Reel	Forward Reel
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	GBG	Bag-In-Box or BIB	Bag-In-Box or BIB is a type of container for the storage and transportation of liquids. It consists of a strong bladder, usually made of aluminium PET film or other plastics seated inside a corrugated fibreboard box. The box and internal bag can be fused
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	GBR	Brick	Brick: A rectangular-shaped, stackable package designed primarily for liquids such as juice or milk.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	GGT	Gable Top	Gable Top: A rectangular-shaped, non-stackable package designed primarily for liquids such as juice or milk.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	GNT	Net	Net: A container of meshwork material made from threads or strips twisted or woven to form a regular pattern with spaces between the threads that is used for holding, carrying, trapping, or confining something.

FDA GUDID Code- Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	GPB	Pallet Box	Pallet Box: A three-dimensional container which either has a pallet platform permanently attached at its base or alternatively requires a platform for its handling and storage as due to its constitution it cannot be handled without it. The characteristics
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	GPP	Peel Pack	Peel Pack: A package used for sterile products which may be torn open without touching the product inside.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	GPU	Packed, Unspecified	Packed, Unspecified: Packaging of the product (or products) is currently not on the list. Use this code when no suitable options are available and only while a Change Request is approved for the proper packaging type.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	HPR	Hamper	Hamper
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	HPT	Hopper Truck	Hopper Truck
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field	Packaging Type Code	HRB	On Hanger or Rack in Boxes	On Hanger or Rack in Boxes



FDA GUDID Code- Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
	at right should be passed to the FDA GUDID.				
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	HRK	Half-Standard Rack	Half-Standard Rack
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	HTB	Half-Standard Tote Bin	Half-Standard Tote Bin
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	INT	Intermediate Container	Intermediate Container
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	JAR	Jar	Jar: A rigid container made of glass, stone, earthenware, plastic or other appropriate material with a large opening, which is used to store products, (e.g., jams, cosmetics).
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	JG	Jug	Jug: A container, normally cylindrical, with a handle and/or a lid or spout for holding and pouring liquids.
Packaging Type	GDSN utilizes the code value, however GUDID currently	Packaging Type Code	KEG	Keg	Keg



FDA GUDID Code- Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
	needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.				
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	KIT	Kit	Kit
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	KRK	Knockdown Rack	Knockdown Rack
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	KTB	Knockdown Tote Bin	Knockdown Tote Bin
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	LAB	Label Tag	Label Tag
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.	Packaging Type Code	LID	Lip/Top	Lip/Top: In packaging, the top or bottom of a container, usually the part that closes the opening; may also be known as cap, over, or top

FDA GUDID Code- Attribute- Code Group	Code Value
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.

GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
Packaging Type Code	LIF	Lifts	Lifts
Packaging Type Code	LNR	Liners	Liners: Any material that separates a product within a container from the basic walls of the container
Packaging Type Code	LOG	Log	Log
Packaging Type Code	LSE	Loose	Loose
Packaging Type Code	LUG	Lug	Lug
Packaging Type Code	LVN	Lift Van	Lift Van

FDA GUDID Code- Attribute- Code Group	Code Value
	at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently

GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
Packaging Type Code	MIX	Mixed Container Types	Mixed Container Types: More than one type of container is included in a shipment (shipment could consist of 3 pieces that include 1 box, 1 crate, and 1 basket)\
Packaging Type Code	ML2	MILVAN	MILVAN: A military owned demountable container that conforms to US and international standards and operates in a centrally controlled fleet for movement of military cargo
Packaging Type Code	MPE	Multipack	Multipack
Packaging Type Code	MRP	Multi-Roll Pack	Multi-Roll Pack
Packaging Type Code	MS2	MSCVAN	MSCVAN: A commercial (leased) or Government-owned shipping container controlled by the Military Sealift Command.
Packaging Type Code	MXD	Mixed	Mixed

FDA GUDID Code- Attribute- Code Group	Code Value
	needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.

GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
Packaging Type Code	NOL	Noil	Noil
Packaging Type Code	PA	Packet	Packet
Packaging Type Code	PAF	Pallet, 4- Way	Pallet – 4 Way: A pallet that permits entry of handling equipment on each of its four sides
Packaging Type Code	PAL	Pail	Pail
Packaging Type Code	PAT	Pallet, 2-way	Pallet - 2 Way: A pallet that permits entry of handling equipment on opposing two of its four sides

FDA GUDID Code- Attribute- Code Group	Code Value
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.

GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
Packaging Type Code	PCK	Packed	Packed - not otherwise specified
Packaging Type Code	PCS	Pieces	Pieces
Packaging Type Code	PIR	Pirns	Pirns
Packaging Type Code	PKG	Package	Package
Packaging Type Code	PLC	Primary Lift Container	Primary Lift Container: The largest (outermost) unitized package or articles secured together that can be handled (usually mechanically) in common shop floor/warehouse applications as a single entity; "primary" indicates preferred or mandatory
Packaging Type Code	PLF	Platform	Platform

FDA GUDID Code- Attribute- Code Group	Code Value
	at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently

GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
Packaging Type Code	PLN	Pipeline	Pipeline
Packaging Type Code	PLT	Pallet	Pallet: A platform used to hold or transport unit loads.
Packaging Type Code	PO	Pouch	Pouch: A preformed, flexible container, generally enclosed with a gusset seal at the bottom of the pack can be shaped/arranged to allow the pack to stand on shelf.
Packaging Type Code	POV	Private Vehicle	Private Vehicle
Packaging Type Code	PRK	Pipe Rack	Pipe Rack
Packaging Type Code	PRT	Partitioning	Partitioning: The proceeds of applying separators or dividers

FDA GUDID Code- Attribute- Code Group	Code Value
	needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.

GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
Packaging Type Code	PUN	Punnet	Punnet
Packaging Type Code	PWT	Plastic-Wrapped Tray	Plastic-Wrapped Tray
Packaging Type Code	RAL	Rail (Semiconductor)	Rail (Semiconductor)
Packaging Type Code	RCK	Rack	A non-specific term identifying a framework or stand for carrying, holding, or storing items. Commonly on wheels and primarily used in the logistical functions to deliver items such as hanging garments, or items on shelves such as dairy products and baker
Packaging Type Code	REL	Reel	Reel: A spool on which thread, wire, film, etc, is wound. Any device on which a material may be wound. Usually has flanged ends and is used for shipping or processing purposes.



FDA GUDID Code- Attribute- Code Group	Code Value
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.

GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
Packaging Type Code	RFT	Reinforcement	Reinforcement: In containers and shipping devices, a component (usually temporary) added to a container for a particular application to lend additional support under severe applications
Packaging Type Code	ROL	Roll	Roll
Packaging Type Code	RVR	Reverse Reel	Reverse Reel
Packaging Type Code	SAK	Sack	Sack
Packaging Type Code	SCS	Suitcase	Suitcase
Packaging Type Code	SHK	Shook	Shook

FDA GUDID Code- Attribute- Code Group	Code Value
	at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently

GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
Packaging Type Code	SHT	Sheet	Sheet: A thin layer of material usually used as a pad for extra protection by isolating/separating tiers or layers of parts within the package
Packaging Type Code	SKD	Skid	Skid
Packaging Type Code	SKE	Skid, elevating or lift truck	Skid, elevating or lift truck
Packaging Type Code	SLP	Slip Sheet	Slip Sheet: Shipping containers utilizing slip sheets, which are cardboard platforms used to hold product for storage or transportation
Packaging Type Code	SLV	Sleeve	Sleeve: A non-rigid container usually made of paper, cardboard or plastic, that is open-ended and is slid over the contents for protection or presentation.
Packaging Type Code	SPI	Spin Cylinders	Spin Cylinders

FDA GUDID Code- Attribute- Code Group	Code Value
	needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.

GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
Packaging Type Code	SPL	Spool	Spool
Packaging Type Code	SPR	Separator/Divider	Separator/Divider: In packaging, any material inserted between tiers or layers of articles to prevent contact and provide protection
Packaging Type Code	SRW	Shrink Wrap	Shrink Wrap: In packaging, a plastic film around an item or group of items which is heated causing the film to shrink, securing the unit integrity. The use of shrunken film to tightly wrap a package or a unit load in order to bind, protect and immobilize
Packaging Type Code	STW	Stretch Wrap	Stretch Wrap: In packaging, a high-tensile plastic film, stretched and wrapped repeatedly around an item or group of items to secure and maintain unit integrity. The use of stretch film to tightly wrap a package or a unit load in order to bind, protect a
Packaging Type Code	SV2	SEAVAN	SEAVAN: A commercial or government-owned (or leased) shipping container which is moved via ocean transportation without wheels attached and is lifted on and off a ship

FDA GUDID Code- Attribute- Code Group	Code Value
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.

GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
Packaging Type Code	TBE	Tube	Tube: A cylindrical container sealed on one end that could be closed with a cap or dispenser on the other end.
Packaging Type Code	TBN	Tote Bin	Tote Bin
Packaging Type Code	TKR	Tank Car	Tank Car
Packaging Type Code	TKT	Tank Truck	Tank Truck
Packaging Type Code	TLD	Intermodal Trailer/Container Load (Rail)	Intermodal Trailer/Container Load (Rail)
Packaging Type Code	TNK	Tank	Tank

FDA GUDID Code- Attribute- Code Group	Code Value
	at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently

GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
Packaging Type Code	TRC	Tierce	Tierce
Packaging Type Code	TRK	Trunk and Chest	Trunk and Chest
Packaging Type Code	TRU	Truck	Truck
Packaging Type Code	TRY	Tray	Tray: A shallow container, which may or may not have a cover, used for displaying or carrying items.
Packaging Type Code	TSS	Trunk, Salesmen Sample	Trunk, Salesmen Sample
Packaging Type Code	TUB	Tub	Tub: Generally, a round flat-bottomed container closed with a large lid, typically used to contain ice

FDA GUDID Code- Attribute- Code Group	Code Value
	needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.

GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
			cream, margarine, sour cream, confections, and other products.
Packaging Type Code	UNP	Unpacked	Unpacked: The item is provided without packaging.
Packaging Type Code	UNT	Unit	Unit
Packaging Type Code	UVQ	Wrapped in Plastic	Wrapped in Plastic
Packaging Type Code	VEH	Vehicles	Vehicles
Packaging Type Code	VIL	Vial	Vial

FDA GUDID Code- Attribute- Code Group	Code Value
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.
Packaging Type	GDSN utilizes the code value, however GUDID currently needs a term for the code. The term in the description field at right should be passed to the FDA GUDID.

GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
Packaging Type Code	VOC	Vehicle in Operating Condition	Vehicle in Operating Condition
Packaging Type Code	VP	Vacuum Packed	Vacuum Packed: Packaging in containers, either rigid or flexible, from which substantially all gases have been removed prior to final sealing of the container.
Packaging Type Code	VPK	Van Pack	Van Pack
Packaging Type Code	WHE	On Own Wheel	On Own Wheel
Packaging Type Code	WLC	Wheeled Carrier	Wheeled Carrier
Packaging Type Code	WRP	Wrapped	Wrapped: The process of enclosing all or part of an item with layers of flexible wrapping material (e.g., for an individually packed ice cream). Does not include items which are shrink-wrapped or vacuum-packed.

FDA GUDID Code- Attribute- Code Group	Code Value
	at right should be passed to the FDA GUDID.
Prescription Use (Rx)	Prescription Use (Rx)
Secondary-DI-Issuing Agency	ICCBA
Secondary-DI-Issuing Agency	GS1
Serial Number	TRUE
Serial Number	TRUE
Serial Number	TRUE
Serial Number	FALSE
Serial Number	FALSE
SizeType	Circumference
SizeType	Depth
SizeType	Device Size Text, specify
SizeType	Catheter Gauge (Formerly French Catheter Gauge)
SizeType	Greatest Diameter
SizeType	Height
SizeType	Length
SizeType	Lumen/Inner Diameter (formerly Lumen Diameter)
SizeType	Needle Gauge
SizeType	Second Greatest Diameter (REMOVED 4/16/2014)
SizeType	Third Greatest Diameter (REMOVED 4/16/2014)
SizeType	Total Volume

GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
Consumer Sales Conditions	PRESCRIPTION_REQUIRED		Trade item may only be sold or dispensed under the direction of a prescription.
Additional Trade Item Identification Type	PENDING		GDSN Change Request (CR) in process to add this code value
Additional Trade Item Identification Type			Not needed as there can only be one GTIN for an item and therefore cannot be a secondary GTIN.
serialNumberLocationCode	MARKED_ON_PACKAGING		Serial number is on the trade item's packaging.
serialNumberLocationCode	MARKED_ON_PACKAGING_INSERT		Serial number is on the trade item's packaging insert.
serialNumberLocationCode	MARKED_ON_TRADE_ITEM		Serial number is on the trade item.
serialNumberLocationCode	NOT_MARKED		The trade item or its packaging is not marked
serialNumberLocationCode	UNKNOWN		Unknown location of marking.
clinicalSizeType	CIRCUMFERENCE	Circumference	
ClinicalSizeType	DEPTH	Depth	
ClinicalSizeType	DEVICE_SIZE_TEXT_SPECIFY	Device Size Text, specify	
ClinicalSizeType	GAUGE (PENDING)	Gauge	GDSN Change Request in process to add this code value
ClinicalSizeType	GREATEST_DIAMETER	Greatest Diameter	
ClinicalSizeType	HEIGHT	Height	
ClinicalSizeType	LENGTH	Length	
ClinicalSizeType	LUMEN/INNER_DIAMETER (PENDING)	Lumen/Inner Diameter	GDSN Change Request in process to add this code value
ClinicalSizeType	NEEDLE_GAUGE	Needle Gauge	
ClinicalSizeType	TOTAL_VOLUME	Total Volume	



FDA GUDID Code- Attribute- Code Group	Code Value
SizeType	Width
SizeType	Angle
SizeType	Area/Surface Area
SizeType	Outer Diameter
SizeType	Pore size
SizeType	Pressure
SizeType	Weight
Sterilization Method	Moist Heat or Steam
Sterilization Method	Radiation
Sterilization Method	Ethylene Oxide
Sterilization Method	Radiation
Sterilization Method	Dry Heat

GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
ClinicalSizeType		Width	
ClinicalSizeType	Angle		GDSN Change Request in process to add this code value
ClinicalSizeType	Area/Surface Area		GDSN Change Request in process to add this code value
ClinicalSizeType	Outer Diameter		GDSN Change Request in process to add this code value
ClinicalSizeType	Pore size		GDSN Change Request in process to add this code value
ClinicalSizeType	Pressure		GDSN Change Request in process to add this code value
ClinicalSizeType	Weight		GDSN Change Request in process to add this code value
Initial Manufacture Sterilization Initial Sterilization Prior to Use	AUTOCLAVE		Autoclave (Steam) is a method of sterilisation that utilizes pressure and heat to achieve a sterile environment.
Initial Manufacture Sterilization Initial Sterilization Prior to Use	BETA_RADIATION		Beta particles are able to penetrate living matter to a certain extent (radiation intensity from a small source of radioactive material decreases as one over the distance squared) and can change the structure of struck molecules.
Initial Manufacture Sterilization Initial Sterilization Prior to Use	ETO_ETHYLENE_OXID E		A gas that is commonly used to sterilize objects sensitive to temperatures greater than 60 °C such as plastics, optics and electrics. Ethylene oxide treatment is generally carried out between 30 °C and 60 °C with relative humidity above 30% and a gas concentration between 200 and 800 mg/L for at least three hours. Ethylene oxide penetrates well, moving through paper, cloth, and some plastic films and is highly effective.
Initial Manufacture Sterilization Initial Sterilization Prior to Use	GAMMA_RADIATION		Gamma rays are very penetrating and are commonly used for sterilization of disposable medical equipment, such as syringes, needles, cannulas and IV sets. Gamma radiation requires bulky shielding for the safety of the operators; they also require storage o
Initial Manufacture Sterilization Initial Sterilization Prior to Use	DRY_HEAT		GDSN Change Request (CR) in process to add this code value

FDA GUDID Code- Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
Sterilization Method	High Intensity Light or Pulse Light	Initial Manufacture Sterilization Initial Sterilization Prior to Use	HIGH_INTENSITY_LIGHT_OR_PULSE_LIGHT		GDSN Change Request (CR) in process to add this code value
Sterilization Method	Microwave Radiation	Initial Manufacture Sterilization Initial Sterilization Prior to Use	MICROWAVE		GDSN Change Request (CR) in process to add this code value
Sterilization Method	Sound Waves	Initial Manufacture Sterilization Initial Sterilization Prior to Use	SOUND_WAVES		GDSN Change Request (CR) in process to add this code value
Sterilization Method	Hydrogen Peroxide	Initial Manufacture Sterilization Initial Sterilization Prior to Use	HYDROGEN_PEROXIDE		Another chemical sterilizing agent. It is relatively non-toxic once diluted to low concentrations (although a dangerous oxidizer at high concentrations), and leaves no residue.
Sterilization Method	Ozone	Initial Manufacture Sterilization Initial Sterilization Prior to Use	OZONE		Is a method often times used in industrial settings to sterilize water and air, as well as a disinfectant for surfaces. It has the benefit of being able to oxidize most organic matter. It is a toxic and unstable gas that must be produced on-site, so it is
Sterilization Method	Peracetic Acid	Initial Manufacture Sterilization Initial Sterilization Prior to Use	PERACETIC_ACID		A chemical in the organic peroxide family. It is a bright, colorless liquid with a characteristic acrid acetic acid type odor. It has a strong oxidizing potential, is highly corrosive, and can explode at temperatures exceeding 110 °C.
Sterilization Method	Ultraviolet Light	Initial Manufacture Sterilization Initial Sterilization Prior to Use	UV_LIGHT		Useful for sterilization of surfaces and some transparent objects. Many objects that are transparent to visible light absorb UV. UV irradiation is routinely used to sterilize the interiors of biological safety cabinets between uses.
Sterilization Method	Chlorine Dioxide	Initial Manufacture Sterilization Initial Sterilization Prior to Use	CHLORINE_DIOXIDE		GDSN Change Request (CR) in process to add this code value
Storage and Handling Type	Storage Environment Atmospheric Pressure	Storage and Handling GDSN Attributes	StorageEnvironmentAtmosphericPressureMaximum OR storageEnvironmentAtmosphericPressureMinimum		

FDA GUDID Code- Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Value	Code Description (where applicable)	Definition
			m		
Storage and Handling Type	Storage Environment Humidity	Storage and Handling GDSN Attributes	StorageHandlingHumidityMaximum OR storageHandlingHumidityMinimum		
Storage and Handling Type	Storage Environment Temperature	Storage and Handling GDSN Attributes	StorageHandlingTemperatureMaximum OR storageHandlingTemperatureMinimum		
Storage and Handling Type	Handling Environment Atmospheric Pressure	Storage and Handling GDSN Attributes	TransportationEnvironmentAtmosphericPressureMaximum OR transportationEnvironmentAtmosphericPressureMinimum		
Storage and Handling Type	Handling Environment Humidity	Storage and Handling GDSN Attributes	TransportationMaximumHumidityMaximum OR transportationMaximumHumidityMinimum		
Storage and Handling Type	Handling Environment Temperature	Storage and Handling GDSN Attributes	TransportationMaximumTemperature OR transportationMinimumTemperature		
<b>Support-Customer Contact Email</b>	Use to provide the Contact Email for GUDID	Communications Channel	EMAIL		N/A
<b>Support-Customer Contact Email</b>	Use to provide the Contact Phone for GUDID	Communications Channel	TELEPHONE		N/A
FDA GUDID Attribute- Device Count		netContent- (Count)	1N	Count	

The following are the Unit of Measures (UoM) which are used by FDA and the corresponding UoM used in GDSN.

FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
UoM- Angle Units of Measure - {Angle}	deg {Degree}	netContent	Count	DD	Degree (Unit of Angel)	A measurement of plane angle, representing 1/360 of a full rotation; one degree is equivalent to $\pi/180$ radians.
UoM- Area Units of Measure- {Area/Surface Area}	[sft_i] {Square foot}	netContent	Area	FTK	Square foot	A square foot is an area of a square whose sides are exactly 1 foot in length.
UoM- Area Units of Measure- {Area/Surface Area}	[sin_i] {Square inch}	netContent	Area	INK	Square inch	A square inch is an area of a square whose sides are exactly 1 inch in length.
UoM- Area Units of Measure- {Area/Surface Area}	cm2 {Square centimeter}	netContent	Area	CMK	Square centimetre	A square centimetre is an area of a square whose sides are exactly 1 centimetre in length.
UoM- Area Units of Measure- {Area/Surface Area}	m2 {Square meter}	netContent	Area	MTK	Square metre	A square metre is an area of a square whose sides are exactly 1 metre in length.
UoM- Area Units of Measure- {Area/Surface Area}	mm2 {Square millimeter}	netContent	Area	MMK	Square millimetre	A square millimetre is an area of a square whose sides are exactly 1 millimetre in length.
UoM- Gauge - French Units of Measure - {Catheter Gauge}	[Ch] {French }	clinicalSizeValue; height; width; depth; and netContent	Dimension	H79	French gauge	The French scale (most correctly abbreviated as Fr, but also often abbreviated as FR or F) is commonly used to measure the catheter size (Circumference is in millimeters), in which 1 Fr = 0.33 mm in diameter. In the French Gauge system as it is also known, the diameter in millimeters of the catheter can be determined by dividing the French size by 3, thus an increasing French size corresponds with a larger diameter catheter. The following equations summarize the relationships: $D(\text{mm}) = \text{Fr}/3$ or $\text{Fr} = D(\text{mm}) * 3$

FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
UoM- Gauge - Needle Units of Measure - {Needle Gauge}	G {Gauge}	clinicalSizeValue		PENDING	Currently no GDSN or UN Recommendation 20 Value for FDA GUDID UoM. A Change Request has been submitted to correct.	
UoM- Length Size Units of Measure - {Circumference}	{ft_i} {Feet}	clinicalSizeValue; height; width; depth; and netContent	Dimension	FOT	Foot	The international foot is defined to be equal to 0.3048 meters.
UoM- Length Size Units of Measure - {Circumference}	{in_i} {Inch}	clinicalSizeValue; height; width; depth; and netContent	Dimension	INH	Inches	An international inch is defined to be equal to 25.4 millimeters.
UoM- Length Size Units of Measure - {Circumference}	{yd_i} {Yard }	clinicalSizeValue; height; width; depth; and netContent	Dimension	YRD	Yard	A yard is It is equal to 3 feet or 36 inches or 0.9144 meter.
UoM- Length Size Units of Measure - {Circumference}	cm {Centimeter}	clinicalSizeValue; height; width; depth; and netContent	Dimension	CMT	Centimetre	A centimetre is equal to one hundredth of a metre.
UoM- Length Size Units of Measure - {Circumference}	dm {Decimeter}	clinicalSizeValue; height; width; depth; and netContent	Dimension	DMT	Decimetre	A decimetre is equal to one tenth of a metre.
UoM- Length Size Units of Measure - {Circumference}	fm {Femtometer}	clinicalSizeValue		A71	Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code A71. A Change Request has been submitted to correct.	
UoM- Length Size Units of Measure - {Circumference}	km {Kilometer}	clinicalSizeValue; height; width; depth; and netContent	Dimension	KMT	Kilometre	A kilometre is one thousand (1000) metres
UoM- Length Size Units of Measure - {Circumference}	m {Meter}	clinicalSizeValue; height; width; depth; and netContent	Dimension	MTR	Metre	The metre is the basic unit of length in the International System of Units (SI).
UoM- Length Size Units of Measure - {Circumference}	mm {Millimeter}	clinicalSizeValue; height; width; depth; and netContent	Dimension	MMT	Millimetre	A millimetre is one thousandth of a metre (0.001)

FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
UoM- Length Size Units of Measure - {Circumference}	nm {Nanometer}	clinicalSizeValue		C45	Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code C45. A Change Request has been submitted to correct.	
UoM- Length Size Units of Measure - {Circumference}	pm {Picometer}	clinicalSizeValue		C52	Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code C52. A Change Request has been submitted to correct.	
UoM- Length Size Units of Measure - {Circumference}	um {Micrometer}	clinicalSizeValue; height; width; depth; and netContent	Dimension	4H	Micrometre	A micrometre is one millionth of a metre, also termed Micron.
UoM- Length Size Units of Measure - {Depth}	{ft_i} {Feet}	clinicalSizeValue; height; width; depth; and netContent	Dimension	FOT	Foot	The international foot is defined to be equal to 0.3048 meters.
UoM- Length Size Units of Measure - {Depth}	{in_i} {Inch}	clinicalSizeValue; height; width; depth; and netContent	Dimension	INH	Inches	An international inch is defined to be equal to 25.4 millimeters.
UoM- Length Size Units of Measure - {Depth}	{yd_i} {Yard }	clinicalSizeValue; height; width; depth; and netContent	Dimension	YRD	Yard	A yard is it is equal to 3 feet or 36 inches or 0.9144 meter.
UoM- Length Size Units of Measure - {Depth}	cm {Centimeter}	clinicalSizeValue; height; width; depth; and netContent	Dimension	CMT	Centimetre	A centimetre is equal to one hundredth of a metre.
UoM- Length Size Units of Measure - {Depth}	dm {Decimeter}	clinicalSizeValue; height; width; depth; and netContent	Dimension	DMT	Decimetre	A decimetre is equal to one tenth of a metre.

FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
UoM- Length Size Units of Measure - {Depth}	fm {Femtometer}	clinicalSizeValue		A71	Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code A71. A Change Request has been submitted to correct.	
UoM- Length Size Units of Measure - {Depth}	km {Kilometer}	clinicalSizeValue; height; width; depth; and netContent	Dimension	KMT	Kilometre	A kilometre is one thousand (1000) metres
UoM- Length Size Units of Measure - {Depth}	m {Meter}	clinicalSizeValue; height; width; depth; and netContent	Dimension	MTR	Metre	The metre is the basic unit of length in the International System of Units (SI).
UoM- Length Size Units of Measure - {Depth}	mm {Millimeter}	clinicalSizeValue; height; width; depth; and netContent	Dimension	MMT	Millimetre	A millimetre is one thousandth of a metre (0.001)
UoM- Length Size Units of Measure - {Depth}	nm {Nanometer}	clinicalSizeValue		C45	Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code C45. A Change Request has been submitted to correct.	
UoM- Length Size Units of Measure - {Depth}	pm {Picometer}	clinicalSizeValue		C52	Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code C52. A Change Request has been submitted to correct.	

FDA GUDID Code-Attribute- Code Group	Code Value
UoM- Length Size Units of Measure - {Depth}	um {Micrometer}
UoM- Length Size Units of Measure - {Height}	{ft_i} {Feet}
UoM- Length Size Units of Measure - {Height}	{in_i} {Inch}
UoM- Length Size Units of Measure - {Height}	{yd_i} {Yard }
UoM- Length Size Units of Measure - {Height}	cm {Centimeter}
UoM- Length Size Units of Measure - {Height}	dm {Decimeter}
UoM- Length Size Units of Measure - {Height}	fm {Femtometer}
UoM- Length Size Units of Measure - {Height}	km {Kilometer}
UoM- Length Size Units of Measure - {Height}	m {Meter}
UoM- Length Size Units of Measure - {Height}	mm {Millimeter}

GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
clinicalSizeValue; height; width; depth; and netContent	Dimension	4H	Micrometre	A micrometre is one millionth of a metre, also termed Micron.
clinicalSizeValue; height; width; depth; and netContent	Dimension	FOT	Foot	The international foot is defined to be equal to 0.3048 meters.
clinicalSizeValue; height; width; depth; and netContent	Dimension	INH	Inches	An international inch is defined to be equal to 25.4 millimeters.
clinicalSizeValue; height; width; depth; and netContent	Dimension	YRD	Yard	A yard is It is equal to 3 feet or 36 inches or 0.9144 meter.
clinicalSizeValue; height; width; depth; and netContent	Dimension	CMT	Centimetre	A centimetre is equal to one hundredth of a metre.
clinicalSizeValue; height; width; depth; and netContent	Dimension	DMT	Decimetre	A decimetre is equal to one tenth of a metre.
clinicalSizeValue		A71	Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code A71. A Change Request has been submitted to correct.	
clinicalSizeValue; height; width; depth; and netContent	Dimension	KMT	Kilometre	A kilometre is one thousand (1000) metres
clinicalSizeValue; height; width; depth; and netContent	Dimension	MTR	Metre	The metre is the basic unit of length in the International System of Units (SI).
clinicalSizeValue; height; width; depth; and netContent	Dimension	MMT	Millimetre	A millimetre is one thousandth of a metre (0.001)



FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
UoM- Length Size Units of Measure - {Height}	nm {Nanometer}	clinicalSizeValue		C45	Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code C45. A Change Request has been submitted to correct.	
UoM- Length Size Units of Measure - {Height}	pm {Picometer}	clinicalSizeValue		C52	Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code C52. A Change Request has been submitted to correct.	
UoM- Length Size Units of Measure - {Height}	um {Micrometer}	clinicalSizeValue; height; width; depth; and netContent	Dimension	4H	Micrometre	A micrometre is one millionth of a metre, also termed Micron.
UoM- Length Size Units of Measure - {Length}	{ft_i} {Feet}	clinicalSizeValue; height; width; depth; and netContent	Dimension	FOT	Foot	The international foot is defined to be equal to 0.3048 meters.
UoM- Length Size Units of Measure - {Length}	{in_i} {Inch}	clinicalSizeValue; height; width; depth; and netContent	Dimension	INH	Inches	An international inch is defined to be equal to 25.4 millimeters.
UoM- Length Size Units of Measure - {Length}	{yd_i} {Yard }	clinicalSizeValue; height; width; depth; and netContent	Dimension	YRD	Yard	A yard is it is equal to 3 feet or 36 inches or 0.9144 meter.
UoM- Length Size Units of Measure - {Length}	cm {Centimeter}	clinicalSizeValue; height; width; depth; and netContent	Dimension	CMT	Centimetre	A centimetre is equal to one hundredth of a metre.
UoM- Length Size Units of Measure - {Length}	dm {Decimeter}	clinicalSizeValue; height; width; depth; and netContent	Dimension	DMT	Decimetre	A decimetre is equal to one tenth of a metre.

FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
UoM- Length Size Units of Measure - {Length}	fm {Femtometer}	clinicalSizeValue		A71	Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code A71. A Change Request has been submitted to correct.	
UoM- Length Size Units of Measure - {Length}	km {Kilometer}	clinicalSizeValue; height; width; depth; and netContent	Dimension	KMT	Kilometre	A kilometre is one thousand (1000) metres
UoM- Length Size Units of Measure - {Length}	m {Meter}	clinicalSizeValue; height; width; depth; and netContent	Dimension	MTR	Metre	The metre is the basic unit of length in the International System of Units (SI).
UoM- Length Size Units of Measure - {Length}	mm {Millimeter}	clinicalSizeValue; height; width; depth; and netContent	Dimension	MMT	Millimetre	A millimetre is one thousandth of a metre (0.001)
UoM- Length Size Units of Measure - {Length}	nm {Nanometer}	clinicalSizeValue		C45	Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code C45. A Change Request has been submitted to correct.	
UoM- Length Size Units of Measure - {Length}	pm {Picometer}	clinicalSizeValue		C52	Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code C52. A Change Request has been submitted to correct.	

FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
UoM- Length Size Units of Measure - {Length}	um {Micrometer}	clinicalSizeValue; height; width; depth; and netContent	Dimension	4H	Micrometre	A micrometre is one millionth of a metre, also termed Micron.
UoM- Length Size Units of Measure - {Lumen/Inner Diameter}	[ft_i] {Feet}	clinicalSizeValue; height; width; depth; and netContent	Dimension	FOT	Foot	The international foot is defined to be equal to 0.3048 meters.
UoM- Length Size Units of Measure - {Lumen/Inner Diameter}	[in_i] {Inch}	clinicalSizeValue; height; width; depth; and netContent	Dimension	INH	Inches	An international inch is defined to be equal to 25.4 millimeters.
UoM- Length Size Units of Measure - {Lumen/Inner Diameter}	[yd_i] {Yard }	clinicalSizeValue; height; width; depth; and netContent	Dimension	YRD	Yard	A yard is It is equal to 3 feet or 36 inches or 0.9144 meter.
UoM- Length Size Units of Measure - {Lumen/Inner Diameter}	cm {Centimeter}	clinicalSizeValue; height; width; depth; and netContent	Dimension	CMT	Centimetre	A centimetre is equal to one hundredth of a metre.
UoM- Length Size Units of Measure - {Lumen/Inner Diameter}	dm {Decimeter}	clinicalSizeValue; height; width; depth; and netContent	Dimension	DMT	Decimetre	A decimetre is equal to one tenth of a metre.
UoM- Length Size Units of Measure - {Lumen/Inner Diameter}	fm {Femtometer}	clinicalSizeValue		A71	Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code A71. A Change Request has been submitted to correct.	
UoM- Length Size Units of Measure - {Lumen/Inner Diameter}	km {Kilometer}	clinicalSizeValue; height; width; depth; and netContent	Dimension	KMT	Kilometre	A kilometre is one thousand (1000) metres
UoM- Length Size Units of Measure - {Lumen/Inner Diameter}	m {Meter}	clinicalSizeValue; height; width; depth; and netContent	Dimension	MTR	Metre	The metre is the basic unit of length in the International System of Units (SI).
UoM- Length Size Units of Measure - {Lumen/Inner Diameter}	mm {Millimeter}	clinicalSizeValue; height; width; depth; and netContent	Dimension	MMT	Millimetre	A millimetre is one thousandth of a metre (0.001)

FDA GUDID Code-Attribute- Code Group	Code Value
UoM- Length Size Units of Measure - {Lumen/Inner Diameter}	nm {Nanometer}
UoM- Length Size Units of Measure - {Lumen/Inner Diameter}	pm {Picometer}
UoM- Length Size Units of Measure - {Lumen/Inner Diameter}	um {Micrometer}
UoM- Length Size Units of Measure - {Outer Diameter}	[ft_i] {Feet}
UoM- Length Size Units of Measure - {Outer Diameter}	[in_i] {Inch}
UoM- Length Size Units of Measure - {Outer Diameter}	[yd_i] {Yard }
UoM- Length Size Units of Measure - {Outer Diameter}	cm {Centimeter}
UoM- Length Size Units of Measure - {Outer Diameter}	dm {Decimeter}

GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
clinicalSizeValue		C45	Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code C45. A Change Request has been submitted to correct.	
clinicalSizeValue		C52	Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code C52. A Change Request has been submitted to correct.	
clinicalSizeValue; height; width; depth; and netContent	Dimension	4H	Micrometre	A micrometre is one millionth of a metre, also termed Micron.
clinicalSizeValue; height; width; depth; and netContent	Dimension	FOT	Foot	The international foot is defined to be equal to 0.3048 meters.
clinicalSizeValue; height; width; depth; and netContent	Dimension	INH	Inches	An international inch is defined to be equal to 25.4 millimeters.
clinicalSizeValue; height; width; depth; and netContent	Dimension	YRD	Yard	A yard is It is equal to 3 feet or 36 inches or 0.9144 meter.
clinicalSizeValue; height; width; depth; and netContent	Dimension	CMT	Centimetre	A centimetre is equal to one hundredth of a metre.
clinicalSizeValue; height; width; depth; and netContent	Dimension	DMT	Decimetre	A decimetre is equal to one tenth of a metre.

FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
UoM- Length Size Units of Measure - {Outer Diameter}	fm {Femtometer}	clinicalSizeValue		A71	Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code A71. A Change Request has been submitted to correct.	
UoM- Length Size Units of Measure - {Outer Diameter}	km {Kilometer}	clinicalSizeValue; height; width; depth; and netContent	Dimension	KMT	Kilometre	A kilometre is one thousand (1000) metres
UoM- Length Size Units of Measure - {Outer Diameter}	m {Meter}	clinicalSizeValue; height; width; depth; and netContent	Dimension	MTR	Metre	The metre is the basic unit of length in the International System of Units (SI).
UoM- Length Size Units of Measure - {Outer Diameter}	mm {Millimeter}	clinicalSizeValue; height; width; depth; and netContent	Dimension	MMT	Millimetre	A millimetre is one thousandth of a metre (0.001)
UoM- Length Size Units of Measure - {Outer Diameter}	nm {Nanometer}	clinicalSizeValue		C45	Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code C45. A Change Request has been submitted to correct.	
UoM- Length Size Units of Measure - {Outer Diameter}	pm {Picometer}	clinicalSizeValue		C52	Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code C52. A Change Request has been submitted to correct.	

FDA GUDID Code-Attribute- Code Group	Code Value
UoM- Length Size Units of Measure - {Outer Diameter}	um {Micrometer}
UoM- Length Size Units of Measure - {Pore Size}	{ft_i} {Feet}
UoM- Length Size Units of Measure - {Pore Size}	{in_i} {Inch}
UoM- Length Size Units of Measure - {Pore Size}	{yd_i} {Yard }
UoM- Length Size Units of Measure - {Pore Size}	cm {Centimeter}
UoM- Length Size Units of Measure - {Pore Size}	dm {Decimeter}
UoM- Length Size Units of Measure - {Pore Size}	fm {Femtometer}
UoM- Length Size Units of Measure - {Pore Size}	km {Kilometer}
UoM- Length Size Units of Measure - {Pore Size}	m {Meter}
UoM- Length Size Units of Measure - {Pore Size}	mm {Millimeter}

GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
clinicalSizeValue; height; width; depth; and netContent	Dimension	4H	Micrometre	A micrometre is one millionth of a metre, also termed Micron.
clinicalSizeValue; height; width; depth; and netContent	Dimension	FOT	Foot	The international foot is defined to be equal to 0.3048 meters.
clinicalSizeValue; height; width; depth; and netContent	Dimension	INH	H29	An international inch is defined to be equal to 25.4 millimeters.
clinicalSizeValue; height; width; depth; and netContent	Dimension	YRD	Yard	A yard is It is equal to 3 feet or 36 inches or 0.9144 meter.
clinicalSizeValue; height; width; depth; and netContent	Dimension	CMT	Centimetre	A centimetre is equal to one hundredth of a metre.
clinicalSizeValue; height; width; depth; and netContent	Dimension	DMT	Decimetre	A decimetre is equal to one tenth of a metre.
clinicalSizeValue		A71	Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code A71. A Change Request has been submitted to correct.	
clinicalSizeValue; height; width; depth; and netContent	Dimension	KMT	J33	A kilometre is one thousand (1000) metres
clinicalSizeValue; height; width; depth; and netContent	Dimension	MTR	J34	The metre is the basic unit of length in the International System of Units (SI).
clinicalSizeValue; height; width; depth; and netContent	Dimension	MMT	MC	A millimetre is one thousandth of a metre (0.001)

FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
UoM- Length Size Units of Measure - {Pore Size}	nm {Nanometer}	clinicalSizeValue		C45	Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code C45. A Change Request has been submitted to correct.	
UoM- Length Size Units of Measure - {Pore Size}	pm {Picometer}	clinicalSizeValue		C52	Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code C52. A Change Request has been submitted to correct.	
UoM- Length Size Units of Measure - {Pore Size}	um {Micrometer}	clinicalSizeValue; height; width; depth; and netContent	Dimension	4H	J35	A micrometre is one millionth of a metre, also termed Micron.
UoM- Pressure Units of Measure- {Pressure }	[psi] {Pound per Square Inch}	storageEnvironmentAtmosphericPressureMaximum + UoM; storageEnvironmentAtmosphericPressureMinimum + UoM; transportationEnvironmentAtmosphericPressureMaximum + UoM; and transportationEnvironmentAtmosphericPressureMinimum + UoM	Pressure	80	Pound per square inch - Absolute	Psia (pound-force per square inch absolute) is a unit of pressure relative to a vacuum (such as that in space). At sea level, Earth's atmosphere actually exerts a pressure of 14.7 psi. Humans do not feel this pressure because internal pressure of liquid in their bodies matches the external pressure. If a pressure gauge is calibrated to read zero in space, then at sea level on Earth it would read 14.7 psi. Thus a reading of 30 psig, on Earth, on a tire gauge represents an absolute pressure of 44.7 psi (lb/in <sup>2</sup> ).

FDA GUDID Code-Attribute- Code Group	Code Value
UoM- Pressure Units of Measure- {Pressure }	Hz {Hertz}
UoM- Pressure Units of Measure- {Pressure }	kPa {KiloPascal}
UoM- Pressure Units of Measure- {Pressure }	mbar {millibar }

GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
netContent	Frequency	HTZ	Hertz	A unit of frequency defined as the number of complete cycles per second; it is the basic unit of frequency in the International System of Units (SI).
clinicalSizeValue		KPA	Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code KPA. A Change Request has been submitted to correct.	
clinicalSizeValue		MBR	Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code MBR. A Change Request has been submitted to correct.	



FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
<p>UoM- Pressure Units of Measure- {Pressure }</p>	<p>mg/{TotalVolume} {Milligram per Total Volume}</p>	<p>clinicalSizeValue</p>		<p>PENDING</p>	<p>Currently no GDSN or UN Recommendation 20 Value for FDA GUDID UoM. A Question is posed to the FDA to clarify which volume they refer to or does it matter. If it does not matter, UN Recommendation 20 has the following to be used and a GDSN Change request would be entered to support- NA, M1, C12, H63, MF, MK, GO.</p>	
<p>UoM- Pressure Units of Measure- {Pressure }</p>	<p>U/L {Units per Liter}</p>	<p>clinicalSizeValue</p>		<p>PENDING</p>	<p>Currently no GDSN or UN Recommendation 20 Value for FDA GUDID UoM. A Question is posed to the FDA to clarify which unit they refer to.</p>	

FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
UoM- Pressure Units of Measure- {Pressure }	ug/{TotalVolume} {Microgram per Total Volume}	clinicalSizeValue		PENDING	Currently no GDSN or UN Recommendation 20 Value for FDA GUDID UoM. A Question is posed to the FDA to clarify which volume they refer to or does it matter. If it does not matter, UN Recommendation 20 has the following to be used and a GDSN Change request would be entered to support- GQ, H29, J33, J34, J35, MC.	
UoM- Storage and Handling Units of Measure - {Handling Environment Atmospheric Pressure}	[degf] {Degrees Fahrenheit}	storageHandlingTemperatureMaximum + UoM; storageHandlingTemperatureMinimum + UoM; transportationMaximumTemperature + UoM; and transportationMinimumTemperature + UoM	Temperature	FAH	Degree Fahrenheit	The Fahrenheit temperature scale, the freezing point of water is 32 degrees Fahrenheit (°F) and the boiling point 212 °F (at standard atmospheric pressure), placing the boiling and freezing points of water exactly 180 degrees apart.
UoM- Storage and Handling Units of Measure - {Handling Environment Atmospheric Pressure}	Cel {Degrees Celsius}	storageHandlingTemperatureMaximum + UoM; storageHandlingTemperatureMinimum + UoM; transportationMaximumTemperature + UoM; and transportationMinimumTemperature + UoM	Temperature	CEL	Degree Celsius	Celsius (also historically known as centigrade) is a temperature scale, the freezing point of water is 0 degrees Celsius (°C) and the boiling point 100 °C (at standard atmospheric pressure), placing the boiling and freezing points of water exactly 100 degrees apart.

FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
UoM- Storage and Handling Units of Measure - {Handling Environment Atmospheric Pressure}	K {Degrees Kelvin}	storageHandlingTemperatureMaximum + UoM; storageHandlingTemperatureMinimum + UoM; transportationMaximumTemperature + UoM; and transportationMinimumTemperature + UoM	Temperature	KEL	Kelvin	Kelvin: a unit of absolute temperature equal to 1/273.16 of the absolute temperature of the triple point of water. One kelvin degree is equal to one Celsius degree.
UoM- Storage and Handling Units of Measure - {Handling Environment Atmospheric Pressure}	kPa {KiloPascal}				Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code KPA. A Change Request has been submitted to correct.	
UoM- Storage and Handling Units of Measure - {Handling Environment Atmospheric Pressure}	Percent {Percent (%) Relative Humidity}	storageHandlingHumidityMaximum + UoM; storageHandlingHumidityMinimum + UoM; transportationHumidityMaximum + UoM; and transportationHumidityMinimum + UoM	Proportion	P1	Percent	A unit of proportion equal to 0.01.
UoM- Storage and Handling Units of Measure - {Handling Environment Humidity}	{degf} {Degrees Fahrenheit}	storageHandlingTemperatureMaximum + UoM; storageHandlingTemperatureMinimum + UoM; transportationMaximumTemperature + UoM; and transportationMinimumTemperature + UoM	Temperature	FAH	Degree Fahrenheit	The Fahrenheit temperature scale, the freezing point of water is 32 degrees Fahrenheit (°F) and the boiling point 212 °F (at standard atmospheric pressure), placing the boiling and freezing points of water exactly 180 degrees apart.

FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
UoM- Storage and Handling Units of Measure - {Handling Environment Humidity}	Cel {Degrees Celsius}	storageHandlingTemperatureMaximum + UoM; storageHandlingTemperatureMinimum + UoM; transportationMaximumTemperature + UoM; and transportationMinimumTemperature + UoM	Temperature	CEL	Degree Celsius	Celsius (also historically known as centigrade) is a temperature scale, the freezing point of water is 0 degrees Celsius (°C) and the boiling point 100 °C (at standard atmospheric pressure), placing the boiling and freezing points of water exactly 100 degrees apart.
UoM- Storage and Handling Units of Measure - {Handling Environment Humidity}	K {Degrees Kelvin}	storageHandlingTemperatureMaximum + UoM; storageHandlingTemperatureMinimum + UoM; transportationMaximumTemperature + UoM; and transportationMinimumTemperature + UoM	Temperature	KEL	Kelvin	Kelvin: a unit of absolute temperature equal to 1/273.16 of the absolute temperature of the triple point of water. One kelvin degree is equal to one Celsius degree.
UoM- Storage and Handling Units of Measure - {Handling Environment Humidity}	kPa {KiloPascal}	clinicalSizeValue		KPA	Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code KPA. A Change Request has been submitted to correct.	
UoM- Storage and Handling Units of Measure - {Handling Environment Humidity}	Percent {Percent (%) Relative Humidity}	storageHandlingHumidityMaximum + UoM; storageHandlingHumidityMinimum + UoM; transportationHumidityMaximum + UoM; and transportationHumidityMinimum + UoM	Proportion	P1	Percent	A unit of proportion equal to 0.01.

FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
UoM- Storage and Handling Units of Measure - {Handling Environment Temperature}	[degf] {Degrees Fahrenheit}	storageHandlingTemperatureMaximum + UoM; storageHandlingTemperatureMinimum + UoM; transportationMaximumTemperature + UoM; and transportationMinimumTemperature + UoM	Temperature	FAH	Degree Fahrenheit	The Fahrenheit temperature scale, the freezing point of water is 32 degrees Fahrenheit (°F) and the boiling point 212 °F (at standard atmospheric pressure), placing the boiling and freezing points of water exactly 180 degrees apart.
UoM- Storage and Handling Units of Measure - {Handling Environment Temperature}	Cel {Degrees Celsius}	storageHandlingTemperatureMaximum + UoM; storageHandlingTemperatureMinimum + UoM; transportationMaximumTemperature + UoM; and transportationMinimumTemperature + UoM	Temperature	CEL	Degree Celsius	Celsius (also historically known as centigrade) is a temperature scale, the freezing point of water is 0 degrees Celsius (°C) and the boiling point 100 °C (at standard atmospheric pressure), placing the boiling and freezing points of water exactly 100 degrees apart.
UoM- Storage and Handling Units of Measure - {Handling Environment Temperature}	K {Degrees Kelvin}	storageHandlingTemperatureMaximum + UoM; storageHandlingTemperatureMinimum + UoM; transportationMaximumTemperature + UoM; and transportationMinimumTemperature + UoM	Temperature	KEL	Kelvin	Kelvin: a unit of absolute temperature equal to 1/273.16 of the absolute temperature of the triple point of water. One kelvin degree is equal to one Celsius degree.
UoM- Storage and Handling Units of Measure - {Handling Environment Temperature}	kPa {KiloPascal}	clinicalSizeValue		KPA	Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code KPA. A Change Request has been submitted to correct.	

FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
UoM- Storage and Handling Units of Measure - {Handling Environment Temperature}	Percent {Percent (%) Relative Humidity}	storageHandlingHumidityMaximum + UoM; storageHandlingHumidityMinimum + UoM; transportationHumidityMaximum + UoM; and transportationHumidityMinimum + UoM	Proportion	P1	Percent	A unit of proportion equal to 0.01.
UoM- Storage and Handling Units of Measure - {Storage Environment Atmospheric Pressure}	{degf} {Degrees Fahrenheit}	storageHandlingTemperatureMaximum + UoM; storageHandlingTemperatureMinimum + UoM; transportationMaximumTemperature + UoM; and transportationMinimumTemperature + UoM	Temperature	FAH	Degree Fahrenheit	The Fahrenheit temperature scale, the freezing point of water is 32 degrees Fahrenheit (°F) and the boiling point 212 °F (at standard atmospheric pressure), placing the boiling and freezing points of water exactly 180 degrees apart.
UoM- Storage and Handling Units of Measure - {Storage Environment Atmospheric Pressure}	Cel. {Degrees Celsius}	storageHandlingTemperatureMaximum + UoM; storageHandlingTemperatureMinimum + UoM; transportationMaximumTemperature + UoM; and transportationMinimumTemperature + UoM	Temperature	CEL	Degree Celsius	Celsius (also historically known as centigrade) is a temperature scale, the freezing point of water is 0 degrees Celsius (°C) and the boiling point 100 °C (at standard atmospheric pressure), placing the boiling and freezing points of water exactly 100 degrees apart.
UoM- Storage and Handling Units of Measure - {Storage Environment Atmospheric Pressure}	K {Degrees Kelvin}	storageHandlingTemperatureMaximum + UoM; storageHandlingTemperatureMinimum + UoM; transportationMaximumTemperature + UoM; and transportationMinimumTemperature + UoM	Temperature	KEL	Kelvin	Kelvin: a unit of absolute temperature equal to 1/273.16 of the absolute temperature of the triple point of water. One kelvin degree is equal to one Celsius degree.

FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
UoM- Storage and Handling Units of Measure - {Storage Environment Atmospheric Pressure}	kPa {KiloPascal}	clinicalSizeValue		KPA	Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code KPA. A Change Request has been submitted to correct.	
UoM- Storage and Handling Units of Measure - {Storage Environment Atmospheric Pressure}	Percent {Percent (%) Relative Humidity}	storageHandlingHumidityMaximum + UoM; storageHandlingHumidityMinimum + UoM; transportationHumidityMaximum + UoM; and transportationHumidityMinimum + UoM	Proportion	P1	Percent	A unit of proportion equal to 0.01.
UoM- Storage and Handling Units of Measure - {Storage Environment Humidity}	[degf] {Degrees Fahrenheit}	storageHandlingTemperatureMaximum + UoM; storageHandlingTemperatureMinimum + UoM; transportationMaximumTemperature + UoM; and transportationMinimumTemperature + UoM	Temperature	FAH	Degree Fahrenheit	The Fahrenheit temperature scale, the freezing point of water is 32 degrees Fahrenheit (°F) and the boiling point 212 °F (at standard atmospheric pressure), placing the boiling and freezing points of water exactly 180 degrees apart.
UoM- Storage and Handling Units of Measure - {Storage Environment Humidity}	Cel {Degrees Celsius}	storageHandlingTemperatureMaximum + UoM; storageHandlingTemperatureMinimum + UoM; transportationMaximumTemperature + UoM; and transportationMinimumTemperature + UoM	Temperature	CEL	Degree Celsius	Celsius (also historically known as centigrade) is a temperature scale, the freezing point of water is 0 degrees Celsius (°C) and the boiling point 100 °C (at standard atmospheric pressure), placing the boiling and freezing points of water exactly 100 degrees apart.

FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
UoM- Storage and Handling Units of Measure - {Storage Environment Humidity}	K {Degrees Kelvin}	storageHandlingTemperatureMaximum + UoM; storageHandlingTemperatureMinimum + UoM; transportationMaximumTemperature + UoM; and transportationMinimumTemperature + UoM	Temperature	KEL	Kelvin	Kelvin: a unit of absolute temperature equal to 1/273.16 of the absolute temperature of the triple point of water. One kelvin degree is equal to one Celsius degree.
UoM- Storage and Handling Units of Measure - {Storage Environment Humidity}	kPa {KiloPascal}	clinicalSizeValue		KPA	Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code KPA. A Change Request has been submitted to correct.	
UoM- Storage and Handling Units of Measure - {Storage Environment Humidity}	Percent {Percent (%) Relative Humidity}	storageHandlingHumidityMaximum + UoM; storageHandlingHumidityMinimum + UoM; transportationHumidityMaximum + UoM; and transportationHumidityMinimum + UoM	Proportion	P1	Percent	A unit of proportion equal to 0.01.
UoM- Storage and Handling Units of Measure - {Storage Environment Temperature}	{degf} {Degrees Fahrenheit}	storageHandlingTemperatureMaximum + UoM; storageHandlingTemperatureMinimum + UoM; transportationMaximumTemperature + UoM; and transportationMinimumTemperature + UoM	Temperature	FAH	Degree Fahrenheit	The Fahrenheit temperature scale, the freezing point of water is 32 degrees Fahrenheit (°F) and the boiling point 212 °F (at standard atmospheric pressure), placing the boiling and freezing points of water exactly 180 degrees apart.



FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
UoM- Storage and Handling Units of Measure - {Storage Environment Temperature}	Cel {Degrees Celsius}	storageHandlingTemperatureMaximum + UoM; storageHandlingTemperatureMinimum + UoM; transportationMaximumTemperature + UoM; and transportationMinimumTemperature + UoM	Temperature	CEL	Degree Celsius	Celsius (also historically known as centigrade) is a temperature scale, the freezing point of water is 0 degrees Celsius (°C) and the boiling point 100 °C (at standard atmospheric pressure), placing the boiling and freezing points of water exactly 100 degrees apart.
UoM- Storage and Handling Units of Measure - {Storage Environment Temperature}	K {Degrees Kelvin}	storageHandlingTemperatureMaximum + UoM; storageHandlingTemperatureMinimum + UoM; transportationMaximumTemperature + UoM; and transportationMinimumTemperature + UoM	Temperature	KEL	Kelvin	Kelvin: a unit of absolute temperature equal to 1/273.16 of the absolute temperature of the triple point of water. One kelvin degree is equal to one Celsius degree.
UoM- Storage and Handling Units of Measure - {Storage Environment Temperature}	kPa {KiloPascal}	clinicalSizeValue		KPA	Currently no GDSN Value for FDA GUDID UoM. UN Recommendation 20 has this as code KPA. A Change Request has been submitted to correct.	
UoM- Storage and Handling Units of Measure - {Storage Environment Temperature}	Percent {Percent (%) Relative Humidity}	storageHandlingHumidityMaximum + UoM; storageHandlingHumidityMinimum + UoM; transportationHumidityMaximum + UoM; and transportationHumidityMinimum + UoM	Proportion	P1	Percent	A unit of proportion equal to 0.01.
UoM- Volume Units of Measure- {Total Volume}	[cin_i] {Cubic Inch}	netContent	Volume	INQ	Cubic inch	A cubic inch is the volume of a cube of side length one inch (0.254 m).
UoM- Volume Units of Measure- {Total Volume}	[cup_us] {Cup}	netContent	Volume	CU	Cup	

FDA GUDID Code-Attribute- Code Group	Code Value
UoM- Volume Units of Measure- (Total Volume)	[foz_us] {Fluid Ounce}
UoM- Volume Units of Measure- (Total Volume)	[gal_us] {Gallon}
UoM- Volume Units of Measure- (Total Volume)	[pt_us] {Pint}
UoM- Volume Units of Measure- (Total Volume)	[qt_us] {Quart}
UoM- Volume Units of Measure- (Total Volume)	cL {Centiliter}
UoM- Volume Units of Measure- (Total Volume)	dL {Deciliter}
UoM- Volume Units of Measure- (Total Volume)	fL {Femtoliter}
UoM- Volume Units of Measure- (Total Volume)	kL {Kiloliter}
UoM- Volume Units of Measure- (Total Volume)	L {Liter}
UoM- Volume Units of Measure- (Total Volume)	mL {Milliliter}

GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
netContent	Volume	OZA	Fluid ounce (US)	A fluid ounce (US) is equal to one sixteenth (1/16) of a US pint or 29.5735295625 millilitres.
netContent	Volume	GLL	Gallon (US)	The U.S. liquid gallon is legally defined as 231 cubic inches, and is equal to exactly 3.785411784 litres or about 0.133680555 cubic feet.
netContent	Volume	PTI	Pint (UK)	A pint (UK) is equal to 1/8 Gallon (UK); used primarily as a measure for beer and cider when sold by the glass.
netContent	Volume	QTD	Quart (US dry)	A US dry quart is equal to 1/32 of a US bushel, exactly 1.101220942715 litres.
netContent	Volume	CLT	centilitre	10 <sup>-5</sup> m <sup>3</sup>
netContent	Volume	DLT	Decilitre	A decilitre is one tenth (1/10) of a litre.
clinicalSizeValue		PENDING	Currently no GDSN or UN Recommendation 20 Value for FDA GUDID UoM. A Change Request has been submitted to correct.	
netContent	Volume	K6	Kilolitre	A kilolitre is one thousand (1000) litres.
netContent	Volume	LTR	Litre	A litre is defined as a special name for a cubic decimetre (1 L = 1 dm <sup>3</sup> = 103 cm <sup>3</sup> ).
netContent	Volume	MLT	Millilitre	A millilitre is one thousandth of a litre (0.001)

FDA GUDID Code-Attribute- Code Group	Code Value
UoM- Volume Units of Measure- {Total Volume}	nL {Nanoliter}
UoM- Volume Units of Measure- {Total Volume}	pL {Picoliter}
UoM- Volume Units of Measure- {Total Volume}	uL {Microliter}
UoM- Weight Units of Measure - {Weight}	[lb_av] {Pound}
UoM- Weight Units of Measure - {Weight}	[ston_av] {Ton }
UoM- Weight Units of Measure - {Weight}	g {Gram}
UoM- Weight Units of Measure - {Weight}	kg {Kilogram}
UoM- Weight Units of Measure - {Weight}	mg {Milligram }
UoM- Weight Units of Measure - {Weight}	t {Metric Ton}
UoM- Weight Units of Measure - {Weight}	ug {Microgram}

GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
clinicalSizeValue		PENDING	Currently no GDSN or UN Recommendation 20 Value for FDA GUDID UoM. A Change Request has been submitted to correct.	
clinicalSizeValue		PENDING	Currently no GDSN or UN Recommendation 20 Value for FDA GUDID UoM. A Change Request has been submitted to correct.	
netContent	Volume	4G	Microlitre	A microlitre is one millionth of a litre
grossWeight; and netContent	Mass	LBR	Pound	The international avoirdupois pound of exactly 0.45359237 kilogram.
grossWeight; and netContent	Mass	STN	Ton (US) or short ton (UK)	Ton (US) = 2000 Lb or 907 Kg
grossWeight; and netContent	Mass	GRM	Gram	A gram is defined as one one-thousandth of the kilogram (1x10-3 kg).
grossWeight; and netContent	Mass	KGM	Kilogram	A unit of mass equal to one thousand grams.
grossWeight; and netContent	Mass	MGM	Milligram	A milligram is one thousandth of a gram (0.001)
grossWeight; and netContent	Mass	TNE	Tonne	Metric ton = 1000 Kg
grossWeight; and netContent	Mass	MC	Microgram	A microgram is one millionth of a gram (0.000001)
netContent	Area	BB	Base box	A unit of area of 112 sheets of tin mil products (tin plate, tin free steel or black plate) 14 by 20 inches, or 31,360 square inches.

FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
		netContent	Area	DMK	Square decimetre	A square decimetre is an area of a square whose sides are exactly 1 decimetre in length.
		netContent	Area	MIK	Square mile	A square mile is an area of a square whose sides are exactly 1 mile in length.
		netContent	Area	SF	Square Foot	An area of a square whose sides are exactly 1 foot in length.
		netContent	Area	SM	Square Metre	A square metre is an area of a square whose sides are exactly 1 metre in length.
		netContent	Area	SY	Square Yard	The area of a square with sides of one yard (three feet, thirty-six inches, 0.9144 metres) in length.
		netContent	Area	YDK	Square Yard	A square yard is the area of a square with sides of one yard (three feet, thirty-six inches, 0.9144 metres) in length
		netContent	Count	15	Stick	
		netContent	Count	2P	Kilobyte	A unit of information equal to 10 <sup>3</sup> (1000) bytes.
		netContent	Count	4L	Megabyte	A unit of information equal to 10 <sup>6</sup> (1000000) bytes.
		netContent	Count	5B	Batch	A unit of count defining the number of batches (batch: quantity of material produced in one operation or number of animals or persons coming at once).
		netContent	Count	AD	Byte	A unit of information equal to 8 bits.
		netContent	Count	AIU	Anti XA Unit	A unit of measure for blood potency. Units for the anti XA activity which is a measure to the anti-coagulating effect at low molecular heparins.
		netContent	Count	AS	Assortment	A unit of count defining the number of assortments (assortment: set of items)

FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
						grouped in a mixed collection).
		netContent	Count	AXU	Anti XA Unit (International Units)	A unit of measure for blood potency. International units for the anti XA activity which is a measure to the anti-coagulating effect at low molecular heparins. A unit of measure for blood potency
		netContent	Count	BQL	Becquerel	The becquerel (symbol Bq) is the SI derived unit of radioactivity. One Bq is defined as the activity of a quantity of radioactive material in which one nucleus decays per second. SI uses the becquerel rather than the second for the unit of activity measure to avoid dangerous mistakes: a measurement in becquerels is proportional to activity, and thus a more dangerous source of radiation gives a higher reading. A measurement in seconds is inversely proportional.
		netContent	Count	CG	Card	A unit of count defining the number of units of card (card: thick stiff paper or cardboard).
		netContent	Count	CHD	Centesimal Hahnemannian Dilution (CH)	CH Centesimal Scale Attenuation - One millilitre (1.0 ml) of the first centesimal liquid attenuation (1C), or one gram (1.0 g) of the first centesimal trituration (1C) represents 0.01 gram (10.0 mg) of the dry crude medicinal substance. Subsequent liquid or solid attenuations are made by serial progression, succussing or triturating one (1) part of the preceding attenuation to 99 parts of the vehicle, and represent the following proportions of active principle (i.e., dried medicinal substance): 2CH = 10-4, 3CH = 10-6.



FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
		netContent	Count	CV	Cover	
		netContent	Count	D63	Book	A unit of count defining the number of books (book: set of items bound together or written document of a material whole).
		netContent	Count	DZ	Dozen	A unit of count defining the number of units in multiples of 12.
		netContent	Count	DZN	Dozen	A unit of count defining the number of units in multiples of 12.
		netContent	Count	E27	Dose	A unit of count defining the number of doses (dose: a definite quantity of a medicine or drug).
		netContent	Count	E34	Gigabyte	A unit of information equal to 109 bytes.
		netContent	Count	E35	Terabyte	A unit of information equal to 10 <sup>12</sup> bytes.
		netContent	Count	E37	Pixel	A unit of count defining the number of pixels (pixel: picture element).
		netContent	Count	E39	Dots per inch	A unit of count defining the number of dots per linear inch as a measure of the resolution or sharpness of a graphic image.
		netContent	Count	E55	Use	A unit of count defining the number of times an object is used.
		netContent	Count	EA	Each	A unit of count defining the number of items regarded as separate units.
		netContent	Count	EV	Envelope	
		netContent	Count	FJ	Sizing Factor	Commonly used to specify an order sizing factor related to a trade item to allow standard condition brackets for a variety of items.
		netContent	Count	GBQ	Gigabecquerel	A unit of activity equal to 109 becquerels.
		netContent	Count	GRO	Gross	A unit of count defining the number of units in multiples of 144 (12 x 12).
		netContent	Count	H87	Piece	A unit of count defining the number of pieces (piece: a single item, article or exemplar).

FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
		netContent	Count	HC	Hundred count	A unit of count defining the number of units counted in multiples of 100.
		netContent	Count	HD	Half dozen	A unit of count defining the number of units in multiple of six (6).
		netContent	Count	KT	Kit	A unit of count defining the number of kits (kit: tub, barrel or pail).
		clinicalSizeValue; and netContent	Count	LK	Link	A unit of distance equal to 0.01 chain.
		netContent	Count	LR	Layer	A unit of count defining the number of layers.
		netContent	Count	MLM	Millesimal (LM)	LM - Fifty Millesimal Scale Of Attenuation One millilitre (1.0 ml) of the first fifty millesimal attenuation (1LM) represents 6.20 x 10 <sup>-11</sup> of dry crude medicinal substance. Impregnate the lactose in a proportion of 1 to 100 beginning with the liquid substance (mother tincture), then triturate. The second and third triturations are carried out in the same way as when starting with solid products.
		netContent	Count	MTC	Mother Tincture	A count of a dry crude medicinal substance. Mother tincture when used for homeopathic preparations are liquid preparations obtained by the solvent action of a suitable vehicle upon raw materials. The raw materials are usually in the fresh form but may be dried. Mother tinctures for homeopathic preparations may also be obtained from plant juices, with, or without the addition of a vehicle.

FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
		netContent	Count	NIU	Number of International Units	A unit of count defining the number of international units. The International Unit is a unit of measurement for the amount of a substance, based on measured biological activity or effect. The unit is used for vitamins, hormones, some medications, vaccines, blood products, and similar biologically active substances
		netContent	Count	PC	Piece	A unit of count defining the number of pieces (piece: a single item, article or exemplar).
		netContent	Count	PD	Pad	A unit of count defining the number of pads (pad: block of paper sheets fastened together at one end).
		clinicalSizeValue; and netContent	Count	PNT	Point	A single unit on a scale of measurement as part of an incentive program or pricing structure used as a means of making a quantitative evaluation.
		netContent	Count	PR	Pair	A unit of count defining the number of pairs (pair: item described by two's).
		netContent	Count	PTN	Portion	
		netContent	Count	QB	Page - hardcopy	A unit of count defining the number of hardcopy pages (hardcopy page: a page rendered as printed or written output on paper, film, or other permanent medium).
		netContent	Count	RL	Roll	
		netContent	Count	SET	Set	A unit of count defining the number of sets (set: a number of objects grouped together).
		netContent	Count	SH	Sheet	
		netContent	Count	SPS	Sample Per Second	
		netContent	Count	ST	Set	A unit of count defining the number of sets (set: a number of objects grouped together).



FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
		netContent	Count	SX	Shipment	A unit of count defining the number of shipments (shipment: an amount of goods shipped or transported).
		netContent	Count	U2	Tablet	A unit of count defining the number of tablets (tablet: a small flat or compressed solid object).
		netContent	Count	UN	Unit	
		netContent	Count	UZ	Fifty Count	
		netContent	Count	V2	Pouch	
		netContent	Count	X_CHD	Centesimal Hahnemannian Dilution (CH)	A count of attenuation steps or dilution levels representing the homeopathic potency of a substance using the Hahnemannian (CH) method of attenuation; commonly denoted as CH1, CH2, CH3, etc. Each centesimal attenuation step represents one part source material combined with 99 parts dilution medium; commonly denoted as C1, C2, C3, etc.
		netContent	Count	X_KVN	Korsakovian (K)	A count of attenuation steps or dilution levels representing the homeopathic potency of a substance using the Korsakovian (K) method of attenuation; commonly denoted as CK1, CK2, CK3, etc. Each centesimal attenuation step represents one part source material combined with 99 parts dilution medium; commonly denoted as C1, C2, C3, etc.
		netContent	Count	X_MLM	Millesimai (LM)	A count of attenuation steps or dilution levels representing the homeopathic potency of a substance where each attenuation step represents one part source material combined with 49,999 parts dilution medium; commonly denoted as LM1, LM2, LM3, etc.

FDA GUDID Code-Attribute- Code Group	Code Value

GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
netContent	Count	X_MTC	Mother tincture (Dry material)	A count of a dry crud medical substance Mother tincture, when used for homeopathic preparations, are liquid preparations obtained by the solvent action of a suitable vehicle upon raw materials. The raw materials (medical substance) are usually in the fresh form but may be dried. Mother tinctures for homeopathic preparations may also be obtained from plant juices, with, or without the addition of a vehicle.
netContent	Count	X_SPS	Sample per second	A unit of count defining the number of samplings takes during a period of time
netContent	Count	Z52	Usage (e.g. in laundry, 24 usage)	
netContent	Currency	DO	Dollars, U.S.	
netContent	Density	23	Grams Per Cubic Centimetre	Grams Per Cubic Centimetre
netContent	Density	GM	Gram per square metre	In the metric system, the density of all types of paper, paperboard, and fabric, is expressed in terms of grams per square meter (g/m <sup>2</sup> ). This quantity is commonly called grammage both in English and French (ISO 536), though many English-speaking countries still refer to the "weight". The term density here is used somewhat incorrectly, as density is mass by volume. More precisely, it is a measure of the area density, areal density, or surface density.

FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
		netContent	Dimension	BF	Board Foot	A specialized unit of measure for the volume of rough lumber (before drying and planing with no adjustments) or planed/surfaced lumber. It is the volume of a one-foot length of a board one foot wide and one inch thick. Some countries utilize the synonym super foot or superficial foot.
		netContent	Dimension	CM	Centimetre	A centimetre is equal to one hundredth of a metre.
		netContent	Dimension	DK	Kilometre	A kilometre is one thousand (1000) metres.
		netContent	Dimension	FT	Feet	
		netContent	Dimension	HL	Hundred Feet	
		netContent	Dimension	IN	Inch	An international inch is defined to be equal to 25.4 millimetres.
		clinicalSizeValue; height; width; depth; and netContent	Dimension	LF	Linear foot	A unit of count defining the number of feet (12-inch) in length of a uniform width object.
		clinicalSizeValue; height; width; depth; and netContent	Dimension	LM	Linear metre	A unit of count defining the number of metres in length of a uniform width object.
		netContent	Dimension	MR	Metre	The metre is the basic unit of length in the International System of Units (SI).
		clinicalSizeValue; height; width; depth; and netContent	Dimension	SMI	Mile (statute mile)	A statute mile of 5,280 feet (exactly 1,609.344 meters).
		netContent	Dimension	TM	Thousand Feet	
		netContent	Dimension	YD	Yard	
		netContent	Energy	BTU	British thermal unit	The British thermal unit (BTU or Btu) is a traditional unit of energy. It is approximately the amount of energy needed to heat one pound of water one degree Fahrenheit. One Btu is equal to about 1.06 kilojoules. It is used in the power, steam generation, heating and air conditioning industries.
		netContent	Energy	D30	Terajoule	A terajoule is 10 <sup>12</sup> joules

FDA GUDID Code-Attribute- Code Group	Code Value

GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
netContent	Energy	D32	Terawatt hour	A terawatt hour is 109 * kilowatt hour or 3.6 petajoules.
netContent	Energy	D70	Calorie - International Table (IT)	A calorie is 1/100 of the amount of energy required to warm one gram of air-free water from 0 °C to 100 °C at standard atmospheric pressure; this is about 4.190 J. Its use is archaic, having been replaced by the SI unit of energy, the joule. However, in many countries it remains in common use as a unit of food energy. In the context of nutrition, and especially food labelling, the calorie is approximately equal to 4.1868 joules (J), and energy values are normally quoted in kilojoules (kJ) and kilocalories (kcal).
netContent	Energy	E14	Kilocalorie (international table)	A unit of energy equal to 1000 calories.
netContent	Energy	GWH	Gigawatt hour	A gigawatt hour is 109 kilowatt hour or 3.6 terajoules.
netContent	Energy	JOU	Joule	A joule is the energy exerted by a force of one newton acting to move an object through a distance of one metre.
netContent	Energy	KJO	Kilojoule	A kilojoule is 1000 joules
netContent	Energy	KWH	Kilowatt hour	A kilowatt hour is a unit of energy equal to 3.6 megajoules. It is also a common commercial unit of electric energy representing the amount of energy delivered at a rate of 1,000 watts over a period of one hour.
netContent	Energy	MWH	Megawatt hour (1000 kW.h)	A unit of energy defining the total amount of bulk energy transferred or consumed.

FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
		netContent	Energy	WHR	Watt hour	The watt-hour is a unit of energy equivalent to one watt of power expended for one hour of time; it is equal to 3.6 kilojoules. The watt-hour is rarely used to express energy in any form other than electrical.
		netContent	Frequency	A86	Gigahertz	A unit of frequency equal to 10 <sup>9</sup> Hertz
		netContent	Frequency	D29	Terahertz	A unit of frequency equal to 10 <sup>12</sup> Hertz
		netContent	Frequency	KHZ	Kilohertz	A unit of frequency equal to 10 <sup>3</sup> Hertz
		netContent	Frequency	MHZ	Megahertz	A unit of frequency equal to 10 <sup>6</sup> Hertz
		netContent	Luminescence	A24	Candela per Square Meter	Candela per Square Meter is the SI base unit of luminous intensity that is, power emitted by a light source in a particular direction, weighted by the luminosity function in square meters. This is also known as nit in some markets.
		netContent	Luminescence	B60	Lumens per Square Meter	
		netContent	Luminescence	LUX	Lux	Lux is the SI unit of illuminance and luminous emittance, measuring luminous flux per unit area.
		grossWeight; and netContent	Mass	26	Actual Ton	
		grossWeight; and netContent	Mass	58	Net kilogram	A unit of mass defining the total number of kilograms after deductions.
		grossWeight; and netContent	Mass	AF	Centigram	
		grossWeight; and netContent	Mass	APZ	Troy ounce or apothecary ounce	The troy ounce is a unit of imperial measure. In the present day it is most commonly used to gauge the weight and therefore the price of precious metals. One troy ounce equals 480 grains or 31.1035 grams.
		grossWeight; and netContent	Mass	C18	Millimole	A millimole is one thousandth of a mole.

FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
		grossWeight; and netContent	Mass	C34	Mole	The mole (symbol mol) is the SI base unit of amount of substance; one of a few units used to measure this physical quantity. A mole will possess mass exactly equal to the substance's molecular or atomic weight in grams. That is to say, a substance's atomic or molecular mass in atomic mass units is the same as its molar mass in grams. Because of this, one can measure the number of moles in a pure substance by weighing it and comparing the result to its molecular or atomic weight
		grossWeight; and netContent	Mass	CGM	Centigram	A centigram is one hundredth (1/100) of a gram
		grossWeight; and netContent	Mass	CW	Hundred Pounds (CWT)	
		grossWeight; and netContent	Mass	CWA	Hundred pound (cwt) / hundred weight (US)	A unit of weight in the U.S. Customary System equal to 100 pounds (45.36 kilograms); also called cental.
		grossWeight; and netContent	Mass	CWI	Hundred weight (UK)	A unit of weight in the British Imperial System equal to 112 pounds (50.80 kilograms); also called quintal.
		grossWeight; and netContent	Mass	D43	Atomic Mass Units (AMU)	Atomic Mass Units
		grossWeight; and netContent	Mass	DG	Decigram	A decigram is one tenth (1/10) of a gram.
		grossWeight; and netContent	Mass	E4	Gross kilogram	A unit of mass defining the total number of kilograms before deductions.
		grossWeight; and netContent	Mass	GR	Gram	One one-thousandth of the kilogram (1×10 <sup>-3</sup> kg).
		grossWeight; and netContent	Mass	GRN	Grain	A grain or troy grain is precisely 64.79891 milligrams. Exactly 7,000 grains per avoirdupois pound.
		grossWeight; and netContent	Mass	GT	Gross Kilogram	A unit of mass defining the total number of kilograms before deductions.
		grossWeight; and netContent	Mass	HGM	Hectogram	A hectogram is one hundred (100) grams

FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
		grossWeight; and netContent	Mass	KG	Kilogram	A unit of mass equal to one thousand grams.
		grossWeight; and netContent	Mass	LB	Pound	The international avoirdupois pound of exactly 0.45359237 kilogram.
		grossWeight; and netContent	Mass	LTN	Ton (UK) or long ton (US)	Ton (UK) = 1016 Kg or 2240 Lb.
		grossWeight; and netContent	Mass	ME	Milligram	A milligram is one thousandth of a gram (0.001).
		grossWeight; and netContent	Mass	MIU	Million International Unit (NIE)	A unit of count defining the number of international units in multiples of 106.
		grossWeight; and netContent	Mass	MP	Metric Ton	
		grossWeight; and netContent	Mass	NGM	Nanogram	One billionth (1/1,000,000,000) of a gram.
		grossWeight; and netContent	Mass	ON	Ounces per square yard	The weight of one square yard of the material expressed in ounces. Commonly used to express the density or weight of all types of paper, paperboard, and fabric, e.g. 20 OZ or 20 Weight denim has an area density of 20 oz/yd <sup>2</sup> . The term density here is used somewhat incorrectly, as density is mass by volume. More precisely, it is a measure of the area density, areal density, or surface density.
		grossWeight; and netContent	Mass	ONZ	Ounce	A unit of mass with several definitions, the most commonly used of which are equal to approximately 30 grams
		grossWeight; and netContent	Mass	PE	Pounds Equivalent	
		grossWeight; and netContent	Mass	PG	Pound Gross	
		grossWeight; and netContent	Mass	PN	Pounds net	
		grossWeight; and netContent	Mass	X_NGM	Nanogram	A nano gram is 10 <sup>-9</sup> gram or a billionth of a gram..
		netContent	Power	KWT	Kilowatt	A kilowatt is one thousand (1000) watts

FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
		netContent	Power	MAW	Megawatt	A unit of power defining the rate of energy transferred or consumed when a current of 1000 amperes flows due to a potential of 1000 volts at unity power factor.
		netContent	Power	WTT	Watt	A watt is a derived unit of power; one watt is equivalent to 1 joule (J) of energy per second.
		storageEnvironmentAtmosphericPressureMaximum + UoM; storageEnvironmentAtmosphericPressureMinimum + UoM; transportationEnvironmentAtmosphericPressureMaximum + UoM; and transportationEnvironmentAtmosphericPressureMinimum + UoM	Pressure	28	Kilogram per square metre	A unit of pressure equal to 9.80665*10-05 Bar
		storageEnvironmentAtmosphericPressureMaximum + UoM; storageEnvironmentAtmosphericPressureMinimum + UoM; transportationEnvironmentAtmosphericPressureMaximum + UoM; and transportationEnvironmentAtmosphericPressureMinimum + UoM	Pressure	64	Pounds per square inch gauge	At sea level, Earth's atmosphere actually exerts a pressure of 14.7 psi. Humans do not feel this pressure because internal pressure of liquid in their bodies matches the external pressure. If a pressure gauge is calibrated to read zero in space, then at sea level on Earth it would read 14.7 psi. Thus a reading of 30 psig, on Earth, on a tire gauge represents an absolute pressure of 44.7 psi (lb/in <sup>2</sup> ).



FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
		storageEnvironmentAtmosphericPressureMaximum + UoM; storageEnvironmentAtmosphericPressureMinimum + UoM; transportationEnvironmentAtmosphericPressureMaximum + UoM; and transportationEnvironmentAtmosphericPressureMinimum + UoM	Pressure	64	Pound per square inch - Gauge	Psig (pound-force per square inch gauge) is a unit of pressure relative to the surrounding atmosphere. At sea level, Earth's atmosphere actually exerts a pressure of 14.7 psi. Humans do not feel this pressure because internal pressure of liquid in their bodies matches the external pressure. If a pressure gauge is calibrated to read zero in space, then at sea level on Earth it would read 14.7 psi. Thus a reading of 30 psig, on Earth, on a tire gauge represents an absolute pressure of 44.7 psi (lb/in <sup>2</sup> ).
		storageEnvironmentAtmosphericPressureMaximum + UoM; storageEnvironmentAtmosphericPressureMinimum + UoM; transportationEnvironmentAtmosphericPressureMaximum + UoM; and transportationEnvironmentAtmosphericPressureMinimum + UoM	Pressure	BAR	Bar (unit of pressure)	The bar is widely used in descriptions of pressure; 1 bar = 100 kilopascals 0.987 atmospheres.
		storageEnvironmentAtmosphericPressureMaximum + UoM; storageEnvironmentAtmosphericPressureMinimum + UoM; transportationEnvironmentAtmosphericPressureMaximum + UoM; and transportationEnvironmentAtmosphericPressureMinimum + UoM	Pressure	BI	Bar	The bar is widely used in descriptions of pressure 1 bar = 100 kilopascals 0.987 atmospheres.

FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
		storageEnvironmentAtmosphericPressureMaximum + UoM; storageEnvironmentAtmosphericPressureMinimum + UoM; transportationEnvironmentAtmosphericPressureMaximum + UoM; and transportationEnvironmentAtmosphericPressureMinimum + UoM	Pressure	D5	Kilogram per square centimetre	A kilogram-force per square centimeter (kgf/cm <sup>2</sup> ), often just kilogram per square centimeter (kg/cm <sup>2</sup> ), or kilopond per square centimeter is a unit of pressure using metric units. Its use is now deprecated; it is not a part of the International System of Units (SI), the modern metric system. The unit is similar to the English unit psi (lbf/in <sup>2</sup> ).
		storageEnvironmentAtmosphericPressureMaximum + UoM; storageEnvironmentAtmosphericPressureMinimum + UoM; transportationEnvironmentAtmosphericPressureMaximum + UoM; and transportationEnvironmentAtmosphericPressureMinimum + UoM	Pressure	FP	Pound per square foot	A non SI unit of Pressure approximately equal to 47.88025 PASCAL's.
		storageEnvironmentAtmosphericPressureMaximum + UoM; storageEnvironmentAtmosphericPressureMinimum + UoM; transportationEnvironmentAtmosphericPressureMaximum + UoM; and transportationEnvironmentAtmosphericPressureMinimum + UoM	Pressure	PAL	Pascal	The pascal (symbol: Pa) is the SI derived unit of pressure, stress, Young's modulus and tensile strength. It is a measure of force per unit area, defined as one newton per square metre.

FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
		storageEnvironmentAtmosphericPressureMaximum + UoM; storageEnvironmentAtmosphericPressureMinimum + UoM; transportationEnvironmentAtmosphericPressureMaximum + UoM; and transportationEnvironmentAtmosphericPressureMinimum + UoM	Pressure	PS	Pound-force per square inch	The pound-force per square inch (symbol: psi or lbf/in <sup>2</sup> or lbf/in <sup>2</sup> ) is a unit of pressure or of stress based on avoirdupois units. It is the pressure resulting from a force of one pound-force applied to an area of one square inch. Other abbreviations are used that append a modifier to "psi". However, the US National Institute of Standards and Technology recommends that, to avoid confusion, any modifiers be instead applied to the quantity being measured rather than the unit of measure [1] For example, "Pg = 100 psi" rather than "P = 100 psig".
		storageHandlingHumidityMaximum + UoM; storageHandlingHumidityMinimum + UoM; transportationHumidityMaximum + UoM; and transportationHumidityMinimum + UoM	Proportion	59	Part per million	A unit of proportion equal to 10 <sup>-6</sup> (ppm).
		netContent	Sound	2N	Decibel	A measurement for sound in air and other gases, relative to 20 micropascals (μPa) = 2×10 <sup>-5</sup> Pa, the quietest sound a human can hear. This is roughly the sound of a mosquito flying 3 metres away. This is often abbreviated to just "dB"; however the correct abbreviation is dB (SPL), indicating decibel for Sound Pressure Level.

FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
		storageHandlingTemperatureMaximum + UoM; storageHandlingTemperatureMinimum + UoM; transportationMaximumTemperature + UoM; and transportationMinimumTemperature + UoM	Temperature	CE	Degrees Celsius	Celsius (also historically known as centigrade) is a temperature scale, the freezing point of water is 0 degrees Celsius (°C) and the boiling point 100 °C (at standard atmospheric pressure), placing the boiling and freezing points of water exactly 100 degrees apart.
		storageHandlingTemperatureMaximum + UoM; storageHandlingTemperatureMinimum + UoM; transportationMaximumTemperature + UoM; and transportationMinimumTemperature + UoM	Temperature	FA	Degrees Fahrenheit	The Fahrenheit temperature scale, the freezing point of water is 32 degrees Fahrenheit (°F) and the boiling point 212 °F (at standard atmospheric pressure), placing the boiling and freezing points of water exactly 180 degrees apart.
		netContent	Time	ANN	Year	Unit of time equal to 365, 25 days.
		netContent	Time	B10	Bit per second	In telecommunications and computing, bitrate (sometimes written bit rate, data rate or as a variable R or fb) is the number of bits that are conveyed or processed per unit of time. The bit rate is quantified using the bits per second (bit/s or bps) unit.
		netContent	Time	C26	Millisecond	A millisecond (from milli- and second; abbreviation: ms) is a thousandth (1/1000) of a second.
		netContent	Time	DA	Days	A day is one three hundreds and sixty fifth (1/365) of a year
		netContent	Time	DAY	Days	A day is one three hundreds and sixty fifth (1/365) of a year
		netContent	Time	HUR	Hour	An hour is a unit of measurement of time of the duration of 60 minutes, or 3600 seconds. It is 1/24 of a median Earth day.
		netContent	Time	MIN	Minute (unit of time)	A minute is a unit of time equal to 1/60th of an hour or 60 seconds
		netContent	Time	MON	Month	Unit of time equal to 1/12 of a year of 365,25 days



FDA GUDID Code-Attribute- Code Group	Code Value

GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
netContent	Volume	C8	Cubic Decimetre	A cubic decimetre is the volume of a cube of side length one decimetre (0.1 m).
netContent	Volume	CC	Cubic Centimetre	A cubic centimetre is the volume of a cube of side length one centimetre (0.01 m) equal to a millilitre.
netContent	Volume	CF	Cubic Foot	A cubic foot is the volume of a cube of side length one foot (0.3048 m).
netContent	Volume	CI	Cubic Inch	A cubic inch is the volume of a cube of side length one inch (0.254 m).
netContent	Volume	CMQ	Cubic centimetre	A cubic centimetre is the volume of a cube of side length one centimetre (0.01 m) equal to a millilitre.
netContent	Volume	CO	Cubic Meters	A cubic metre is the volume of a cube of side length one metre.
netContent	Volume	CR	Cubic Meter	
netContent	Volume	DMQ	Cubic decimetre	A cubic decimetre is the volume of a cube of side length one decimetre (0.1 m)
netContent	Volume	DRA	Dram (US)	The dram (archaic spelling drachm) was historically both a coin and a weight. Currently it is both a small mass in the Apothecaries' system of weights and a small unit of volume. This unit is called more correctly fluid dram or in contraction also fluidram. The term also refers to the fluid dram, a measure of capacity equal 1/8 of a fluid ounce, which means it is exactly equal to 3.696 691 195 312 5 mL in the United States.







FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
		netContent		BQ	Becquerel	The becquerel (symbol Bq) is the SI derived unit of radioactivity. One Bq is defined as the activity of a quantity of radioactive material in which one nucleus decays per second. SI uses the becquerel rather than the second for the unit of activity measure to avoid dangerous mistakes: a measurement in becquerels is proportional to activity, and thus a more dangerous source of radiation gives a higher reading. A measurement in seconds is inversely proportional.
		netContent		BR	Barrel	
		netContent		BX	Box	
		netContent		CA	Case	
		netContent		CN	Can	
		netContent		CQ	Cartridge	
		netContent		CT	Carton	
		netContent		DR	Drum	
		netContent		DS	Display	
		netContent		ELU	ELISA Units	Enzyme-linked immunosorbent assay unit, is always associated with a product and a method.
		netContent		FH	Micromole	One millionth (10 <sup>-6</sup> ) of a mole.
		netContent		HEP	Histamine Equivalent Prick	Histamine equivalent prick testing for allergen.
		netContent		JR	Jar	
		netContent		KE	Keg	
		netContent		KIU	Kallikrein inactivator unit.	Kallikrein Inactivator Unit per Milliliter definition: An arbitrary unit of a kallikrein inactivator concentration equal to the concentration at which one milliliter of the mixture contains one unit of the kallikrein inactivator

FDA GUDID Code-Attribute- Code Group	Code Value	GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
		netContent		KO	Milliequivalence caustic potash per gram of product	A unit of count defining the number of milligrams of potassium hydroxide per gram of product as a measure of the concentration of potassium hydroxide in the product.
		netContent		KVN	Korsakovian (K)	K Centesimal Scale of Attenuation - One millilitre (1.0 ml) of the first centesimal liquid attenuation (1C), or one gram (1.0 g) of the first centesimal trituration (1C) represents 0.01 gram (10.0 mg) of the dry crude medicinal substance. Subsequent liquid or solid attenuations are made by serial progression, successing or triturating one (1) part of the preceding attenuation to 99 parts of the vehicle, and represent the following proportions of active principle (i.e., dried medicinal substance): 2CH = 10 <sup>-4</sup> , 3CH = 10 <sup>-6</sup> .
		netContent		MEQ	mEq or milliequivalents	Milliequivalents of solute per liter of solvent (or milliNormal where mEq/L = mN). This is especially common for measurement of compounds in biological fluids for instance, the healthy level of potassium in the blood of a human is defined between 3.5 and 5.0 mEq/L.
		netContent		MX	Mod Pallet (Mixed)	
		netContent		NT	Trailer	
		netContent		PA	Pail	
		netContent		PFU	Plaque Forming unit(s)	Plaque Forming unit(s)
		netContent		PH	Pack	
		netContent		PK	Package	
		netContent		PL	Pallet	

FDA GUDID Code-Attribute- Code Group	Code Value

GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
netContent		PPC	Pixels Per Centimetre	A unit of count defining the number of pixels per linear centimetre as a measurement of the resolution of devices in various contexts typically computer displays, image scanners or digital camera image sensors.
netContent		PPI	Pixels Per Inch	A unit of count defining the number of pixels per linear inch (PPI) as a measurement of the resolution of devices in various contexts typically computer displays, image scanners or digital camera image sensors.
netContent		PRS	Potential Renal Solute Load	Refers to all solutes of endogenous or dietary origin that require excretion by the kidneys. Potential renal solute load (PRSL) refers to solutes of dietary origin that would need to be excreted in the urine if none were diverted into synthesis of new tissue and none were lost through nonrenal routes. This is very important to be able to transmit for infant formulas.
netContent		SQE	SQ-E	Number of allergens based on the SQ-E unit
netContent		TE	Tote	
netContent		TK	Tank	
netContent		TY	Tray	
netContent		X_PPC	Pixel per centimetre	A unit of count defining the number of pixels per linear centimetre as a measurement of the resolution of devices in various contexts; typically computer displays, image scanners or digital camera image sensors.

FDA GUDID Code- Attribute- Code Group	Code Value

GS1 GDSN Attribute	GS1 GDSN Code Group	Code Value	Description	Definition
netContent		X_PPI	Pixel per inch	A unit of count defining the number of pixels per linear inch (PPI) as a measurement of the resolution of devices in various contexts; typically computer displays, image scanners or digital camera image sensors.
netContent		Z51	Application (e.g. in hair colorant, 6 applications)	

## 6. Guidance on populating values

This section provides guidance on how to populate each of the GS1 GDSN attributes to meet the requirements of the FDA GUDID attribute list. The choice of attributes in this guidance is related to the GUDID to GDSN Mapping provided in section 4. The guidance is ordered according in line with the order as presented from the FDA documentation.

### 1. Issuing Agency

#### FDA GUDID

Description	Organization accredited by FDA to operate a system for the issuance of UDIs.
Data Entry Notes	Choose a value from the drop down <b>LOV</b> (Webtool)
Edit Rules After Grace Period	Cannot edit, add or delete after the Grace Period
Required?	<b>Required</b>
Data Type & Length	<b>NA</b>
Entry List of Values (LOV)	GS1, HIBCC, ICCBBA
New DI Trigger?	YES
Public/Private Status	PUBLIC

#### GS1 GDSN

Attribute Name	N/A- LOGICAL POPUALTION
Definition	N/A
Data Type	N/A
GDSN Required	N/A

#### Population Guidance (below)

LOGICAL POPULATION- On the outbound GUDID Message by the Data Pool. Will use the value "GS1" in all GDSN instances. By using GDSN, the GTIN of the lowest level of the hierarchy will become the Primary DI. By using a GTIN as the Primary DI, this will require the issuing agency to be GS1.

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute cannot be changed. Many of the data elements are locked and can no longer be edited.

2. Primary DI#

FDA GUDID

Description	An identifier that is the main (primary) lookup for a medical device and meets the requirements to uniquely identify a device through its distribution and use. The primary DI number will be located on the base package, which is the lowest package level of a medical device containing a full UDI. For medical devices without packaging, the primary DI number and full UDI may be on the device itself.
Data Entry Notes	<p>Enter the Device Identifier (DI) Number. Data type and field length are determined by the individual Issuing Agency structure.</p> <p>GS1: Numeric (Num.), with 14 digits</p> <p>HIBCC: Alphanumeric (Alphanum.), with 6-23 characters</p> <p>ICCBBA: Alphanumeric, with 10 or 16 characters</p>
Edit Rules After Grace Period	None (NO edit, add, or delete are allowed)
Required?	Required
Data Type & Length	<p>Type: Num. or Alphanum.</p> <p>Length: min-6, max-23*</p> <p>*defined by Issuing Agency structure.</p>
Entry List of Values (LOV)	NA
New DI Trigger?	YES
Public/Private Status	Public
<b>GS1 GDSN</b>	
Attribute Name	globalTradeItemNumber
Definition-	A particular Global trade item Number, a numerical value used to uniquely identify a trade item. A trade item is any trade item (trade item or service) upon which there is a need to retrieve pre-defined information and that may be planned, priced, ordered, delivered and or invoiced at any point in any supply chain.
Data Type	Identifier (14 digits)
GDSN Required	MANDATORY

Population Guidance (below)

This is one of the key elements in GDSN and is required for the use of GDSN. By using GDSN to provide data to the GUDID, the GTIN will always be the Primary DI. All other issuing agency identification will be published as secondary.

Once published, a 7-day grace period begins. During the grace period, most attribute can be edited. After the grace period ends on day 8, this attribute can not be changed. Many of the data elements are locked and can no longer be edited.

### 3. Device Count

#### FDA GUDID

Description	Number of medical devices in the base package.
Data Entry Notes	Enter the number of devices. Example: Base Package = Box of 100 gloves; Primary DI = 101; Device Count = 100.
Edit Rules After Grace Period	None (NO edit, add, or delete are allowed)
Required?	Required
Data Type & Length	Type: Num. Length: 7
Entry List of Values (LOV)	NA
New DI Trigger?	YES
Public/Private Status	Public

#### GS1 GDSN

Attribute Name	netContent & UoM
Definition-	The amount of the trade item contained by a package, usually as claimed on the label. For example, Water 750ml - net content = "750 MLT"; 20 count pack of diapers, net content = "20 ea." In case of multi-pack, indicates the net content of the total trade item. For fixed value trade items use the value claimed on the package, to avoid variable fill rate issue that arises with some trade item which are sold by volume or weight, and whose actual content may vary slightly from batch to batch. In case of variable quantity trade items, indicates the average quantity.
Data Type	Numeric + Code List
GDSN Required	N/A

#### Population Guidance (below)

The net content attribute is a measurement attribute which is a number and a corresponding qualifier representing the unit of measure (UoM). The unit of measure code values are from the United Nations Recommendation 20 Code List (UN Rec 20).

For GDSN, net content is required when the attribute is `TradeItemAConsumerUnit` is populated with a value of TRUE. This attribute refers to if an item is the unit of end consumption. **There can be more than one instance of this attribute populated.**

**For the GUDID value for Device Count, the data pool will publish the instance with the qualifier of "1N" from all of the netContent values provided. When transferring data from the GDSN message to the SPL message for the FDA GUDID, an instance of netContent with a UoM using the code 1N must exist.**

It is important to note that if the Device Count is greater than 1 (>1), then a Unit of Use DI is required to be provided in the GUDID.

**Relevant examples of how to populate are:**

- **Pack of 6 syringes, where the pack is the device (Primary DI). In this example, netContent would be populated with "6 1N" for a device count of 6.**

- An assay with 5 tests, where the Assay is the device (Primary DI). In this example, netContent would be populated with "1 1N" for a device count of 1. The assay can not be split apart, however a secondary netContent (for GDS Recipients) could be "5 Z52"

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can not be changed. Many of the data elements are locked and can no longer be edited.



#### 4. Unit of Use DI# Number

##### FDA GUDID

**Description** An identifier assigned to an individual medical device when a UDI is not labelled on the individual device at the level of its unit of use. Its purpose is to associate the use of a device to/on a patient.

**Data Entry Notes** **Enter the Unit of Use DI Number.**  
**Unit of Use DI is an identifier used by hospital staff and Materials Management to account for a single device when the UDI is labeled on a higher level of packaging. The Unit of Use DI does not appear on the label.**  
**Data type and field length are determined by the individual Issuing Agency structure.**  
**GS1: Numeric (Num.), with 14 digits**  
**HIBCC: Alphanumeric (Alphanum.), with 6-23 characters**  
**ICCBBA: Alphanumeric, with 10 or 16 characters**  
**If Device Count = 1, cannot add Unit of Use DI Number.**

**Edit Rules After Grace Period** **Edit (Editing of entered data is allowed)**  
**Required?** **Conditionally Required\* \*If Device Count >1**  
**Data Type & Length** **Type: Num. or Alphanum.**  
**Length: min-6, max-23\***  
**\*defined by Issuing Agency structure.**

**Entry List of Values (LOV)** **NA**  
**New DI Trigger?** **NO**  
**Public/Private Status** **Public**

##### GS1GDSN

**Attribute Name** fDAUnitOfUseGTIN  
**Definition-** GTIN of a unit of use, as defined by the FDA. This is a lower level unit which is contained in the Trade Item.  
**Data Type** GTIN  
**GDSN Required** N/A

##### Population Guidance (below)

If the Device Count is greater than 1 (>1), the unit of use DI# is required for population in the GUDID.

This attribute is a temporary attribute (AVP) in GDSN. It will be deployed into the GDSN Schema in 2016-17 into a final solution. This final solution will be part of the GDSN solution for "Level below Each" (LBE).

## 5. Labeler DUNS Number

### FDA GUDID

Description	Business number issued by Dun & Bradstreet (D&B) that is used to associate the Labeler (Company) name and address to a given version of model of a device in GUDID.
Data Entry Notes	Choose appropriate DUNS Number from drop down LOV. (Webtool)  To ensure data consistency for the GUDID, DUNS number submitted to the GUDID should associate to the company name that appears on the device label; ideally the address associated with the DUNS number should also match the address on the device label, but since address is not displayed to the GUDID public user, this is not a requirement for data consistency.  All edits to information connected to the Labeler DUNS Number must be done through Dun & Bradstreet. No edits of DUNS information will be permitted in the GUDID.
Edit Rules After Grace Period	Edit (Editing of entered data is allowed)*  *Other Labeler DUNS listed to your GUDID account can be selected. No Edit (Editing of entered data is allowed)s of DUNS info will be permitted.
Required?	Required
Data Type & Length	NA
Entry List of Values (LOV)	Labeler DUNS LOV (Webtool)
New DI Trigger?	NO
Public/Private Status	Private

### GS1 GDSN

Attribute Name    Pair of attributes in combination

- a. additionalPartyIdentification\type
- b. additionalPartyIdentification\value

#### Definition

- a. Identification of a party by use of a code other than the Global Location Number.
- b. A party identifier that is in addition to the GLN.

#### Data Type

- a. Code List (Multiple Occurrence)
- b. Text (Multiple Occurrence)

GDSN Required    OPTIONAL, however if one of the pair of attributes is populated both attributes must be populated.

#### Population Guidance (below)

The GUDID is asking for a DUNS number for the Labeler. This value will be for the Company as listed on the label. For GDSN, the Labeler is equivalent to the Brand Owner.

Population of this value can be accomplished by populating the code values "DUNS" or "DUNS\_PLUS\_FOUR" in the GDSN attribute Additional Party Identification\type tied to the attribute Brand Owner GLN. The actual "DUNS" or "DUNS\_PLUS\_FOUR" number can then be populated in the GDSN attribute Additional Party Identification\value. The number populated in Additional Party Identification\value will be populated in GUDID as the Labeler DUNS Number.

The FDA will utilize the Labeler DUNS to retrieve the company name and address from D&B. Should the FDA GUDID display an incorrect address, the Labeler must contact D&B to have necessary corrections made.

According to the FDA, the address information retrieved from D&B must match the "Manufactured By" statement on the device or its packaging. The "Manufactured By" statement refers to the entity responsible for the label, its contents and any regulatory filings. This entity may or may not be the "Manufactured At" location. The "Manufactured At" location is the actual facility or facilities where the device is produced or assembled. A device can have more than one "Manufactured At" location, but should only have one "Manufactured By" entity.

## 6. Company Name

### FDA GUDID

Description	Company name associated with the labeler DUNS Number entered in the DI Record.
Data Entry Notes	Auto populated based on the Labeler DUNS Number The labeler company name submitted to the GUDID should match the company name on the device label.
Edit Rules After Grace Period	NA (data element is not able to be changed directly; most are 'auto-populated' fields whose information depends on another data element).
Required?	Auto Populated
Data Type & Length	NA
Entry List of Values (LOV)	NA
New DI Trigger?	NA
Public/Private Status	Public

### GS1 GDSN

Attribute Name	N/A
Definition	N/A
Data Type	N/A
GDSN Required	N/A

### Population Guidance (below)

The FDA will populate this information into the GUDID based on information from D&B based on the Labeler DUNS # provided. If the information is not correct, D&B should be contacted to facilitate correcting the data.

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can only be changed with Dunn and Bradstreet (D&B). Many of the data elements are locked and can no longer be edited.

7. Company Physical Address

FDA GUDID

Description	Company physical address associated with the labeler DUNS Number entered in the DI Record.
Data Entry Notes	Auto populated based on the Labeler DUNS Number Ideally, this address should match the labeler address as shown on the device label but since this data element is not be displayed to the GUDID public user, this is not a requirement for data consistency.
Edit Rules After Grace Period	NA (data element is not able to be changed directly; most are 'auto-populated' fields whose information depends on another data element)
Required?	Auto Populated
Data Type & Length	NA
Entry List of Values (LOV)	NA
New DI Trigger?	NA
Public/Private Status	Private

GS1 GDSN

Attribute Name	N/A
Definition	N/A
Data Type	N/A
GDSN Required	N/A

Population Guidance (Below)

The FDA will populate this information into the GUDID based on information from D&B based on the Labeler DUNS # provided. If the information is not correct, D&B should be contacted to facilitate correcting the data.

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can only be changed with Dunn and Bradstreet (D&B). Many of the data elements are locked and can no longer be edited.

8. Brand Name

FDA GUDID

Description

The Proprietary/Trade/Brand name of the medical device as used in device labeling or in the catalog. This information may 1) be on a label attached to a durable device, 2) be on a package of a disposable device, or 3) appear in labeling materials of an implantable device. The brand name is the name that is typically registered with USPTO and have the ® and/or TM symbol.

Data Entry Notes

Enter the Brand Name.

Only symbols, ® and ™ will be supported for the current production release of GUDID. NOTE: per Edit Rules, you will not be able to change ® or ™ (if entered) after the Grace Period.

Enter NA if the device does not have a Brand Name.

Edit Rules After Grace Period

None (NO edit, add, or delete are allowed)

Required?

Required

Data Type & Length

Type: Alphanumeric.

Length: 80

Entry List of Values (LOV)

NA

New DI Trigger?

YES

Public/Private Status

Public

GS1 GDSN

Attribute Name

brandName

Definition

The recognizable name used by a brand owner to uniquely identify a line of trade item or services. This is recognizable by the consumer.

Data Type

Text (1-35 characters)

GDSN Required

MANDATORY

Population Guidance (below)

This should be the most recognizable brand on the package/trade item. If there is no brand on the package/trade item, this should be the brand name under which the item is sold.

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute cannot be changed. Many of the data elements are locked and can no longer be edited.

9. Version or Model Number

FDA GUDID

Description

The version or model found on the device label or accompanying packaging used to identify a category or design of a device. The version or model identifies all devices that have specifications, performance, size, and composition within limits set by the labeler.

Data Entry Notes

Enter the Version or Model.

Version/Model can be any distinguishing string of letters and/or numbers.

Catalog Number can be entered if device does not currently have a Version or Model. If the device does not have a version, model or catalog number, enter a concept that can be used to identify all devices that have specifications, performance, size, and composition within limits set by the labeler.

Edit Rules After Grace Period

None (NO edit, add, or delete are allowed)

Required?

Required

Data Type & Length

Type: Alphanum.

Length: 40

Entry List of Values (LOV)

NA

New DI Trigger?

YES

Public/Private Status

Public

GS1 GDSN

Attribute Name

Pair of attributes in combination

- a. additionalTradeItemIdentification\type
- b. additionalTradeItemIdentification\value

Definition-

- a. Type of the identification system that is being used as an alternative to the Global Trade Item Number.
- b. Alternative means to the Global Trade Item Number to identify a trade item.

Data Type

- a. Code List (Multiple Occurrence)
- b. Text (Multiple Occurrence)

GDSN Required –

OPTIONAL, however if one of the pair is populated the other must be populated.

Population Guidance (below)

The GUDID is asking for a Model Number for the device. This can be accomplished by the population of the code value "MODEL\_NUMBER" in the GDSN attribute additionalPartyIdentification/type. The actual Model Number can then be populated in the GUDID using the associated additionalPartyIdentification/value(s).

The code value of MODEL\_NUMBER is defined as- (Definition for GDSN Major Release 3.x in 2016) - The additional Trade Item Identification value populated is an identification number, which defines the configuration of the product in addition to the Item number. This is typically printed or otherwise attached to an item. In electronics, this number is typically found around or near a serial number.

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute cannot be changed. Many of the data elements are locked and can no longer be edited.



10. Catalog Number

FDA GUDID

Description –	The catalog, reference, or product number found on the device label or accompanying packaging to identify a particular product.
Data Entry Notes	Enter the Catalog or Reference Number. Catalog/Reference number can also serve as Version/Model if it represents the devices that have specifications, performance, size, and composition within limits set by the labeler.
Edit Rules After Grace Period	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)
Required?	Optional
Data Type & Length	Type: Alphanum. Length: 40
Entry List of Values (LOV)	NA
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Attribute Name	Pair of attributes in combination
a. additionalTradeItemIdentification\type	
b. additionalTradeItemIdentification\value	

Definition

- a. Type of the identification system that is being used as an alternative to the Global Trade Item Number.
- b. Alternative means to the Global Trade Item Number to identify a trade item.

Data Type

- a. Code List (Multiple Occurrence)
- b. Text (Multiple Occurrence)

GDSN Required                      OPTIONAL, however if one of the pair is populated the other must be populated.

Population Guidance (below)

The GUDID is asking for a **Catalog** Number for the device. This can be accomplished by the population of the code value "SUPPLIER\_ASSIGNED" in the GDSN attribute additionalPartyIdentification/type. The actual **Catalog** Number can then be populated in the GUDID using the associated additionalPartyIdentification\value(s).

The code value of SUPPLIER\_ASSIGNED is defined as- (Definition for GDSN Major Release 3.x in 2016) - The additional Trade Item Identification value populated has been developed and assigned by the party which provides service(s) and/or manufactures or otherwise has possession of the goods and consigns or makes them available in trade. This number is a base model or style number assigned to the product and may be the

same for several GTINs where they are variations of each other. For example a coffee mug with 3 GTINs one each for the brown mug, the white mug, and the black mug might all be the supplier assigned number of AB123. Use of this value is recommended in the absence of a Model Number or Manufacturer's Part Number.

11. Device Description (max 2000 characters)

FDA GUDID

Description –	Additional relevant information about the device that is not already captured as a distinct GUDID data attribute.
Data Entry Notes	<b>Enter device description.</b> <b>Device description should include any description found on the device label to support user comparison of the device label to the GUDID device record. Otherwise, include any additional description or text found in the device labeling.</b>
Edit Rules After Grace Period	<b>Add (Addition of new data is allowed)</b> <b>Delete (Deletion of entered data is allowed)</b> <b>Edit (Editing of entered data is allowed)</b>
Required?	<b>Optional</b>
Data Type & Length	<b>Type: Alphanum.</b> <b>Length: 2000</b>
Entry List of Values (LOV)	<b>NA</b>
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Attribute Name- Pair of attributes in combination

- a. tradeItemDescription
- b. additionalTradeItemDescription\text

Definition

a. An understandable and useable description of a trade item using brand and other descriptors. This attribute is filled with as little abbreviation as possible while keeping to a reasonable length. Free form text field, this data element is repeatable for each language used and must be associated with a valid ISO language code. Field length is 178 characters. This should be a meaningful description of the trade item with full spelling to facilitate message processing. Retailers can use this description as the base to fully understand the brand, flavour, scent etc. of the specific GTIN in order to accurately create a product description as needed for their internal systems. Examples:

1. GS1 Brand Base Invisible Solid Deodorant AP Stick Spring Breeze
2. GS1 Brand Laundry Detergent Liquid Compact Regular Instant Stain 1
3. GS1 Brand Hair Colour Liquid Light to Medium Blonde

b. Additional variants necessary to communicate to the industry to help define the product. Multiple variants can be established for each GTIN.

Data Type

- a. Text (Language Qualifier) (1 to 178 Characters)
- b. Text (1-350 characters)

GDSN Required                      OPTIONAL

### Population Guidance (below)

These two attributes will be concatenated together into one value when provided to the GUDID. The concatenation of these two descriptions will provide the best description available as some labellers might have used only one of the two fields. If only one of the attributes is populated in GDSN, only that value will be populated in the GUDID.

12. DI Record Publish Date (mm/dd/yyyy)

FDA GUDID

Description –	Indicates the date the DI Record gets published and is available via Public Search.
Data Entry Notes –	<p>Choose date from calendar or manually enter date in new format (yyyy-mm-dd).</p> <p>This date determines the Grace Period; the 7 calendar days start the day after the DI Record Publish Date. This date should be set in the future to allow time to ensure accurate data entry.</p> <p>We recommend you set this date in the future, but 7 days prior to any compliance deadline. (Drop down is for Webtool only)</p>
Edit Rules After Grace Period	Cannot edit, add, or delete after Published.
Required?	Required
Data Type & Length	Type: Num. (date format) Length: 10
Entry List of Values (LOV)	NA
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Temporary population until final GDSN deployment-

Attribute Name	fDAGUDIDPublishDate
Definition-	The date upon which the Trade Item can be published by the FDA Global Unique Device Identifier Database (FDA GUDID) in their public facing systems. Until this date, the product information may reside in the FDA GUDID, but will not be visible to the public. This data is not changeable.
Data Type	Date Time (CCYY-MM-DDTHH:MM:SS)
GDSN Required	REQUIRED

Population Guidance (below)

This attribute has a temporary attribute (AVP) in GDSN- fDAGUDIDPublishDate. It will be deployed into the GDSN Schema in 2016-17 into a final solution. The final solution will be relationship dependent which allows for a different yet specific value to be provided for each UDIDs.

This attribute can not be changed or edited once the date has been reached. For example if the date is populated as 20140920, then after 9/9/2014, this date can not be edited.

For GDSN, most data pools will auto-populate this date for the manufacturer. However, if a date is populated, that date will not be overwritten.

The Labeler will need to pay particular attention to this date. On this date, the device information will be published by the FDA to the public GUDID site. Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends, on day 8, many of the data elements are locked and can no longer be edited.

If the current date is equal to or greater than the GUDID Publication Date (fdAGUDIDPublishDate [AVP] or uDIDPublishDate in GDSN), then the Commercial Distribution Status will be set to "In Commercial Distribution" automatically by the FDA.

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can not be changed. Many of the data elements are locked and can no longer be edited.

13. Commercial Distribution End Date (mm/dd/yyyy)

FDA GUDID

Description Indicates the date the device is no longer held or offered for sale. See 21 CFR 807.3(b) for exceptions. The device may or may not still be available for purchase in the marketplace.

Data Entry Notes Choose date from calendar or manually enter date in new format (yyyy-mm-dd). (Drop down is for Webtool only)

Edit Rules After Grace Period Add (Addition of new data is allowed)  
Delete (Deletion of entered data is allowed)  
Edit (Editing of entered data is allowed)

Required? Optional

Data Type & Length Type: Num. (date format)  
Length: 10

Entry List of Values (LOV) NA

New DI Trigger? NO

Public/Private Status Public

GS1 GDSN

Attribute Name lastShipDate

Definition Indicates the latest date that the trade item can be shipped. This is independent of any specific ship-from location.

Data Type Date Time (CCYY-MM-DDTHH:MM:SS)

GDSN Required OPTIONAL

Population Guidance (below)

This date signals that a trade item will no longer be in distribution from the Labeler.

If the current date is equal to or greater than the GUDID Commercial Distribution End Date (lastShipDate in GDSN), then the Commercial Distribution Status will be set to "Not in Commercial Distribution" automatically by the FDA.

14. Commercial Distribution Status

FDA GUDID

Description –	Indicates whether the device is in commercial distribution as defined under 21 CFR 807.3(b).
Data Entry Notes	Auto populated based on Commercial Distribution End Date. If no Commercial Distribution End Date is entered, the status is 'In Commercial Distribution'
'Edit Rules After Grace Period	NA (data element is not able to be changed directly; most are 'auto-populated' fields whose information depends on another data element)
Required?	Auto Populated
Data Type & Length	NA
Entry List of Values (LOV)	In Commercial Distribution; Not in Commercial Distribution
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Attribute Name	Derived by the FDA GUDID based on effectiveDate and lastShipDate
Definition	N/A
Data Type	N/A
GDSN Required	N/A

Population Guidance (below)

If the current date is equal to or greater than the GUDID Publication Date (fDAGUDIDPublishDate [AVP] or uDIDPublishDate effectiveDate in GDSN), then the Commercial Distribution Status will be set to “In Commercial Distribution” automatically by the FDA. If the current date is equal to or greater than the GUDID Commercial Distribution End Date (lastShipDate in GDSN), then the Commercial Distribution Status will be set to “Not in Commercial Distribution” automatically by the FDA.



15. Device Subject to Direct Marking (DM), but Exempt

FDA GUDID

Description –	The device is exempt from Direct Marking requirements under 21 CFR 801.45.
Data Entry Notes	<p>Select checkbox if appropriate. (Webtool)</p> <p>Labeler should select the checkbox “Device Subject to Direct Marking (DM), but Exempt” only if the device: (1) is intended to be used more than once and (2) is intended to be reprocessed before each use, but also (3) meets any one of the exception criteria outlined under 21 CFR 801.45(d). If the device is not required to be directly marked under 21 CFR 801.45(a), then this box should not be checked.</p>
Edit Rules After Grace Period	<p>Add (Addition of new data is allowed)</p> <p>Delete (Deletion of entered data is allowed)</p> <p>Edit (Editing of entered data is allowed)</p>
Required?	Conditionally Required* *If device is subject to 801.45
Data Type & Length	Type: Boolean
Entry List of Values (LOV)	NA
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Temporary population until final GDSN deployment-

isTradelItemExemptFromDirectPartMarking

Definition-	Indicator signifying the trade item is exempt from direct identification marking according to regulation or regulatory filings within the target market.
Data Type	Boolean
GDSN Required	Optional
Final Deployment Attribute Name	isTradelItemExemptFromDirectPartMarking
Definition-	Indicator signifying the trade item is exempt from direct identification marking according to regulation or regulatory filings within the target market.
Data Type	Boolean
GDSN Required	Optional

Population Guidance (below)

This value should default to FALSE, unless a Labeler has an exemption and specifically changes the flag to TRUE.

This attribute is a temporary attribute (AVP) in GDSN. It will be deployed into the GDSN Schema in 2016-17 into a final solution.

16. DPM DI Different from Primary DI

FDA GUDID

Description –	Indicates that the DM DI Number is different than the Primary DI Number.
Data Entry Notes	Select checkbox if appropriate. (WebTool)
Edit Rules After Grace Period	<b>Add (Addition of new data is allowed)</b> <b>Delete (Deletion of entered data is allowed)</b> <b>Edit (Editing of entered data is allowed)</b>
Required?	<b>Conditionally Required* *If device is subject to 801.45</b>
Data Type & Length	<b>Type: Boolean</b>
Entry List of Values (LOV)	<b>NA</b>
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Attribute Name	N/A
Definition	N/A
Data Type	N/A
GDSN Required	N/A

Population Guidance (below)

LOGICAL POPULATION- (Logical BOOLEAN value of “TRUE” from the population of a value of “DIRECT\_PART\_MARKING” in GDSN Attribute additionalTradeItemIdentification\type). This GUDID attribute is a Boolean and as such requires a “TRUE” or “FALSE” flag as a value. If there is a value populated for the GDSN attribute combination of additionalTradeItemIdentification\type of “DIRECT\_PART\_MARK”, and an associated additionalTradeItemIdentification\value, then the logical value for the GUDID is “TRUE”, else this value is “FALSE”.

17. DPM DI Number

FDA GUDID

Description	An identifier that is marked directly on the medical device and is different than the Primary DI Number; only applicable to devices subject to Direct Marking requirements under 21 CFR 801.45.
Data Entry Notes	<p><b>Enter Direct Marking DI Number.</b></p> <p><b>Data type and field length are determined by the individual Issuing Agency structure.</b></p> <p><b>GS1: Numeric (Num.), with 14 digits</b></p> <p><b>HIBCC: Alphanumeric (Alphanum.), with 6-23 characters</b></p> <p><b>ICCBBA: Alphanumeric, with 10 or 16 characters</b></p>
Edit Rules After Grace Period	<p><b>Add (Addition of new data is allowed)</b></p> <p><b>Delete (Deletion of entered data is allowed)</b></p> <p><b>Edit (Editing of entered data is allowed)</b></p>
Required?	<b>Conditionally Required* *If device is subject to 801.45 and 'DM DI Different from Primary DI' is checked</b>
Data Type & Length	<p><b>Type:</b></p> <p><b>Num. or Alphanum.</b></p> <p><b>Length: min-6, max-23*</b></p> <p><b>*defined by Issuing Agency structure.</b></p>
Entry List of Values (LOV)	<b>NA</b>
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Temporary population until final GDSN deployment-  
directPartMarking

Definition	This is a number or marking placed directly on the medical device.
Data Type	Text
GDSN Required	Optional
Final Deployment Attribute Name	Pair of attributes in combination
	<ul style="list-style-type: none"> <li>a. additionalTradeItemIdentificaton\type</li> <li>b. additionalTradeItemIdentificaton\value</li> </ul>

Definition

- a. Type of the identification system that is being used as an alternative to the Global Trade Item Number.
- b. Alternative means to the Global Trade Item Number to identify a trade item.

Data Type

- a. Code List (Multiple Occurrence)

## b. Text (Multiple Occurrence)

GDSN Required

OPTIONAL, however if one is populated the other must also be populated.

## Population Guidance (below)

This should only be populated if:

- a) there is a Direct Part Mark on the Device

**AND**

- b) the DI# used in the Direct Part Mark is
- NOT**
- the Primary DI#

This attribute has a temporary attribute (AVP) in GDSN- directPartMarking. It will be deployed into the GDSN Schema in 2016-17 into a final solution.

Population of the GDSN Attribute additionalTradeltemIdentificaton\type with a value of "DIRECT\_PART\_MARK" will allow for the appropriate additionalTradeltemIdentificaton\value to be populated. This attribute pair can be repeated for as many DPM DI#s the item might have. The value populated in the GDSN attribute additionalTradeltemIdentificaton\type attribute associated with the additionalTradeltemIdentificaton\value ("DIRECT\_PART\_MARK") is what will be populated in the GUDID.

This group of attributes will be used to provide several sets of information and as such will be repeated as a group. GUDID attributes using this group of attributes are Version or Model Number, Catalog Number, Secondary DI Number, and FDA Listing Number.

18. Secondary DI Issuing Agency

FDA GUDID

Description	Name of Secondary DI Issuing agency.
Data Entry Notes	Choose a value from the <b>drop down LOV.</b> (Webtool)
Edit Rules After Grace Period	<b>None (NO edit, add, or delete are allowed)</b>
Required?	<b>Optional</b>
Data Type & Length	<b>NA</b>
Entry List of Values (LOV)	GS1; HIBCC; ICCBBA; NHRIC
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Attribute Name	additionalTradeItemIdentification\type
Definition	Type of the identification system that is being used as an alternative to the Global Trade Item Number.
Data Type	Code List
GDSN Required	OPTIONAL (Multiple Occurrence)

Population Guidance (below)

The GS1 General Specifications stipulate that a Trade Item can only have one GTIN. As the GTIN is the primary DI# for an item using GDSN to provide data to the GUDID, a GTIN using GS1 as the issuing agency can not be a secondary DI#. However, the item might have another issuing agency's item number standard in use. Using the GDSN attribute, additionalTradeItemIdentification\type, these other issuing agency identifiers can be provided. Currently, the GDSN attribute has code values for other issuing agencies which would have an associated additionalTradeItemIdentification\value provided to the GUDID. If a value is populated through GDSN for an issuing agency using the attribute additionalTradeItemIdentification\type it will be provided to the GUDID as a secondary DI. The codes available for the Secondary DI Issuing Agency are "HIBC", and "ICCBBA". The population of one of these additionalTradeItemIdentification\type values will denote the appropriate issuing agency code value for GUDID.

This attribute is required if a value is populated for additionalTradeItemIdentification\value.

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can not be changed. Many of the data elements are locked and can no longer be edited.

This group attributes will be used to provide several sets of information and as such will be repeated as a group. GUDID attributes using this group of attributes are Version or Model Number, Catalog Number, Secondary DI Number, and FDA Listing Number.

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can not be changed. Many of the data elements are locked and can no longer be edited.

19. Secondary DI Number

FDA GUDID

Description –	An identifier that is an alternate (secondary) lookup for a medical device that is issued from a different issuing agency than the primary DI. Under 21 CFR 830.40(a), only one device identifier from any particular system for the issuance of UDIs may be used to identify a particular version or model of a device.
Data Entry Notes –	<p>Enter Secondary DI Number.</p> <p>If your product is labeled with a UDI and barcode from more than one issuing agency (for regulatory or marketing reasons), you must choose one issuing agency system as the Primary DI and enter the other issuing agency information here, as a Secondary DI.</p> <p>Data type and field length are determined by the individual Issuing Agency structure.</p> <p>GS1: Numeric (Num.), with 14 digits</p> <p>HIBCC: Alphanumeric (Alphanum.), with 6-23 characters</p> <p>ICCBBA: Alphanumeric, with 10 or 16 characters</p>
Edit Rules After Grace Period	None (NO edit, add, or delete are allowed)
Required?	Optional
Data Type & Length	<p>Type:</p> <p>Num. or Alphanum.</p> <p>Length: min-6, max-23*</p> <p>*defined by Issuing Agency structure.</p>
Entry List of Values (LOV)	NA
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Attribute Name	additionalTradeItemIdentificaton\value
Definition	Alternative means to the Global Trade Item Number to identify a trade item.
Data Type	Text
GDSN Required	OPTIONAL (Multiple Occurrence)

Population Guidance

The GS1 General Specifications stipulate that a Trade Item can only have one GTIN. As the GTIN is the primary DI# for an item using GDSN to provide data to the GUDID, a GTIN using GS1 as the issuing agency can not be a secondary DI#. However, the item might have another issuing agency's item number standard in use. Using the GDSN attribute, additionalTradeItemIdentificaton\value, these other issuing agency identifiers can be provided. If a value is populated through GDSN for an issuing agency using the attribute additionalTradeItemIdentificaton\type it will be provided to the GUDID as a secondary DI. The population of one of the additionalTradeItemIdentificaton\type values

for an issuing agency will denote the appropriate issuing agency code value for GUDID for which the value populated in this attribute is relevant.

This attribute is required if a value is populated for additionalTradeItemIdentification\type.

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can not be changed. Many of the data elements are locked and can no longer be edited.

This group of attributes will be used to provide several sets of information and as such will be repeated as a group. GUDID attributes using this group of attributes are Version or Model Number, Catalog Number, Secondary DI Number, and FDA Listing Number.

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can not be changed. Many of the data elements are locked and can no longer be edited.

20. Package DI Number

FDA GUDID

Description	A device identifier for the package configuration that contains multiple units of the base package (does not include shipping containers).
Data Entry Notes	<p>Enter Package DI Number.</p> <p>Data type and field length are determined by the individual Issuing Agency structure.</p> <p>GS1: Numeric (Num.), with 14 digits</p> <p>HIBCC: Alphanumeric (Alphanum.), with 6-23 characters</p> <p>ICCBBA: Alphanumeric, with 10 or 16 characters</p> <p>Examples:</p> <p>Box of Gloves = DI 101</p> <p>4 Boxes of Gloves (DI 101) in a Carton = Package DI 201 (the UDI on the Carton)</p> <p>5 Cartons (Pkg DI 201) in a Case = Package DI 301 (the UDI on the Case)</p> <p>10 Boxes of Gloves (DI 101) in a Carton = Package DI 202 (the UDI on the Carton).</p>
Edit Rules After Grace Period Required?	<p>Add (Addition of new data is allowed)</p> <p>Conditionally Required*</p> <p>*If device is available in higher levels of packaging</p>
Data Type & Length	<p>Type:</p> <p>Num. or Alphanum.</p> <p>Length: min-6, max-23*</p> <p>*defined by Issuing Agency structure.</p>
Entry List of Values (LOV)	NA
New DI Trigger?	NO
Public/Private Status	Public
GS1 GDSN	
Attribute Name-	globalTradeItemNumber (hierarchy levels where isTradeItemABaseUnit is FALSE)
Definition-	A particular Global trade item Number, a numerical value used to uniquely identify a trade item. A trade item is any trade item (trade item or service) upon which there is a need to retrieve pre-defined information and that may be planned, priced, ordered, delivered and or invoiced at any point in any supply chain.
Data Type	Identifier (14 digits)
GDSN Required-	DEPENDENT (not populated where isTradeItemABaseUnit is TRUE)



Population Guidance (below)

The GUDID Package attributes are populated as a group and can not be entered as single elements in the message. These attributes are:

- Package DI Number
- Quantity per Package
- Contains DI Package
- Package Type
- Package Discontinue Date

All packages must be entered. If a new package level is created, it is to be added to the GUDID as part of the Primary DI to which it is applicable.

This GDSN attribute references a GTIN in the hierarchy above the primary DI. This would be, or is one of, the “parent(s)” of the primary DI. See the example below.

In GDSN, the following is provided.

Hierarchy Number 1

globalTradeItemNumber	tradeItemUnitDescriptor	ChildTradeItem/globalTradeItemNumber	quantityofNextLowerLevelTradeItem	Notes
2061414111111c	CASE	1061414111111c	5	5 cartons in a case
1061414111111c	PACK_OR_INNER_PACK	0061414111111c	4	4 boxes in a carton
0061414111111c	BASE_UNIT_OR_EACH	N/A	N/A	1 Box of Gloves

Hierarchy Number 2

globalTradeItemNumber	tradeItemUnitDescriptor	ChildTradeItem/globalTradeItemNumber	quantityofNextLowerLevelTradeItem	Notes
4061414111111c	CASE	3061414111111c	2	2 cartons in a case
3061414111111c	PACK_OR_INNER_PACK	0061414111111c	10	10 boxes in a carton
0061414111111c	BASE_UNIT_OR_EACH	N/A	N/A	1 Box of Gloves

This is converted to the following for population in the GUDID.

Package DI Number	Quantity per package	Contains DI Package	Notes
1061414111111c	4	0061414111111c	Indicates there are 4 eaches in the pack
2061414111111c	5	3061414111111c	Indicates there are 5 packs in the case
3061414111111c	10	0061414111111c	Indicates there are 10 eaches in the pack
4061414111111c	2	3061414111111c	Indicates there are 2 packs in the case

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can not be deleted.

21. Quantity per package

FDA GUDID

Description	The number of packages with a unique primary DI within a given packaging configuration.
Data Entry Notes	<p>Enter the number of devices per package.</p> <p>The quantity of a package configuration must be &gt;1.</p> <p>Examples:</p> <p>Package – Carton, Pkg DI 201 contains 4 boxes of DI 101; the quantity per package is 4.</p> <p>Package – Case, Pkg DI 301 contains 5 cartons of Pkg DI 201; the quantity per package is 5.</p> <p>Package – Carton, Pkg DI 202 contains 10 boxes of DI 101; the quantity per package is 10.</p>
Edit Rules After Grace Period Required?	<p>Add (Addition of new data is allowed)</p> <p>Conditionally Required*</p> <p>*If Package DI is entered</p>
Data Type & Length	<p>Type: Num.</p> <p>Length: 9</p>
Entry List of Values (LOV)	NA
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Attribute Name	quantityofNextLowerLevelTradeItem
Definition –	The number of one child trade item (as identified by the association of ChildTradeItem class to TradeItemIdentification class) contained by the parent trade item. The child trade item must be in the hierarchy level immediately below the parent trade item.
Data Type	Integer
GDSN Required	DEPENDENT (not populated where isTradeItemABaseUnit is TRUE)

Population Guidance (below)

The GUDID Package attributes are populated as a group and can not be entered as single elements in the message. These attributes are:

- Package DI Number
- Quantity per Package
- Contains DI Package
- Package Type
- Package Discontinue Date

All packages must be entered. If a new package level is created, it is to be added to the GUDID as part of the Primary DI to which it is applicable.

This GDSN attribute references the quantity of the child trade item (GUDID- Contains DI Package), which is contained in the GTIN (GUDID- Package DI Number). See the example below.

In GDSN, the following is provided.

Hierarchy Number 1

globalTradeItemNumber	tradeItemUnitDescriptor	ChildTradeItem/globalTradeItemNumber	quantityofNextLowerLevelTradeItem	Notes
2061414111111c	CASE	1061414111111c	5	5 cartons in a case
1061414111111c	PACK_OR_INNER_PACK	0061414111111c	4	4 boxes in a carton
0061414111111c	BASE_UNIT_OR_EACH	N/A	N/A	1 Box of Gloves

Hierarchy Number 2

globalTradeItemNumber	tradeItemUnitDescriptor	ChildTradeItem/globalTradeItemNumber	quantityofNextLowerLevelTradeItem	Notes
4061414111111c	CASE	3061414111111c	2	2 cartons in a case
3061414111111c	PACK_OR_INNER_PACK	0061414111111c	10	10 boxes in a carton
0061414111111c	BASE_UNIT_OR_EACH	N/A	N/A	1 Box of Gloves

This is converted to the following for population in the GUDID.

Package DI Number	Quantity per package	Contains DI Package	Notes
1061414111111c	4	0061414111111c	Indicates there are 4 eaches in the pack
2061414111111c	5	3061414111111c	Indicates there are 5 packs in the case
3061414111111c	10	0061414111111c	Indicates there are 10 eaches in the pack
4061414111111c	2	3061414111111c	Indicates there are 2 packs in the case

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can not be deleted.

## 22. Contains DI Package

### FDA GUDID

Description	The Primary DI for the base package or the Package DI for any lower level package configuration contained within a given package configuration.
Data Entry Notes	Choose a value from the drop down <b>LOV</b> . (Webtool) <b>Examples:</b> Package DI 201 (Carton) contains base package DI 101. Package DI 202 (Carton) contains base package DI 101. Package DI 301 contains lower level Package DI 201 (Carton).
Edit Rules After Grace Period	Add (Addition of new data is allowed)
Required?	Conditionally Required* *If Package DI is entered
Data Type & Length	NA
Entry List of Values (LOV)	DI numbers; base package and all lower levels of packaging
New DI Trigger?	NO
Public/Private Status	Public

### GS1 GDSN

Attribute Name	ChildTradeItem\globalTradeItemNumber
Definition	A particular Global trade item Number, a numerical value used to uniquely identify a trade item. A trade item is any trade item (trade item or service) upon which there is a need to retrieve pre-defined information and that may be planned, priced, ordered, delivered and or invoiced at any point in any supply chain.
Data Type	Identifier (14 digits)
GDSN Required	DEPENDENT

### Population Guidance (below)

The GUDID Package attributes are populated as a group and can not be entered as single elements in the message. These attributes are:

- Package DI Number
- Quantity per Package
- Contains DI Package
- Package Type
- Package Discontinue Date

All packages must be entered. If a new package level is created, it is to be added to the GUDID as part of the Primary DI to which it is applicable.

This GDSN attribute references the quantity of the child trade item (GUDID- Contains DI Package) which is contained in the GTIN (GUDID- Package DI Number). See the example below.

This GDSN attribute references the hierarchy level which is the next level below, or Child of, the globalTradeitemNumber (GUDID- Package DI Number). See the example below.

In GDSN, the following is provided.

**Hierarchy Number 1**

globalTradeItemNumber	tradeItemUnitDescriptor	ChildTradeItem/globalTradeItemNumber	quantityofNextLowerLevelTradeItem	Notes
2061414111111c	CASE	1061414111111c	5	5 cartons in a case
1061414111111c	PACK_OR_INNER_PACK	0061414111111c	4	4 boxes in a carton
0061414111111c	BASE_UNIT_OR_EACH	N/A	N/A	1 Box of Gloves

**Hierarchy Number 2**

globalTradeItemNumber	tradeItemUnitDescriptor	ChildTradeItem/globalTradeItemNumber	quantityofNextLowerLevelTradeItem	Notes
4061414111111c	CASE	3061414111111c	2	2 cartons in a case
3061414111111c	PACK_OR_INNER_PACK	0061414111111c	10	10 boxes in a carton
0061414111111c	BASE_UNIT_OR_EACH	N/A	N/A	1 Box of Gloves

This is converted to the following for population in the GUDID.

Package DI Number	Quantity per package	Contains DI Package	Notes
1061414111111c	4	0061414111111c	Indicates there are 4 eaches in the pack
2061414111111c	5	3061414111111c	Indicates there are 5 packs in the case
3061414111111c	10	0061414111111c	Indicates there are 10 eaches in the pack
4061414111111c	2	3061414111111c	Indicates there are 2 packs in the case

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can not be deleted.

23. Package Type

FDA GUDID

Description	Text to describe the outer packaging of the product and enables users to understand higher level packaging configurations.
Data Entry Notes	<p>Enter name or description of package.</p> <p>This field is free text. There is no implied definition or standard quantity to any package name.</p>
Edit Rules After Grace Period	Add (Addition of new data is allowed)
Required?	Optional
Data Type & Length	<p>Type: Alphanum.</p> <p>Length: 20</p>
Entry List of Values (LOV)	NA
New DI Trigger?	NO
Public/Private Status	Private

GS1 GDSN

Attribute Name	packagingTypeCode
Definition	The code identifying the type of package used as a container of the trade item.
Data Type	Text (1-3 characters)
GDSN Required	Optional

Population Guidance (below)

The GDSN attribute is a code list and is mapped to the values needed for the GUDID. In GDSN the packaging type code is a 3 character code to identify the type of packaging used for the globalTradeItemNumber. In this case, this value refers to the globalTradeItemNumber which is being used to populate the GUDID Package DI Number. The GUDID is asking for a descriptive term and not the code. There is a mapping list from which the data pools can populate the appropriate descriptive term to publish to the GUDID.

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute cannot be deleted.

## 24. Package Discontinue Date

### FDA GUDID

Description	Indicates the date this particular package configuration is discontinued by the Labeler.
Data Entry Notes	Choose date from calendar or manually enter in format (yyyy-mm-dd).  Discontinuation of a package is directly related to the discontinuation of the primary DI of the base package. However, a package can also be discontinued without the discontinuation of the base package.
Edit Rules After Grace Period Required?	Add (Addition of new data is allowed)  Conditionally Required*  *If Package DI Number and Commercial Distribution End Date are entered, must also enter Package Discontinue Date
Data Type & Length	Type: Num. (date format)  Length: 10
Entry List of Values (LOV)	NA
New DI Trigger?	NO
Public/Private Status	Public

### GS1 GDSN

Attribute Name	discontinuedDate
Definition	Communicate the date on which the trade item is no longer to be manufactured. Allows the reuse of the GTIN after 48 months with the explicit exception of Apparel, being 30 months and the implicit exception for specialty products (e.g., steel beams).
Data Type	Date Time (CCYY-MM-DDTHH:MM:SS)
GDSN Required	Optional

### Population Guidance (below)

This attribute is populated from the globalTradeItemNumber which is being used to populate the GUDID Package DI Number. This date is the date when the Package DI has been discontinued or removed from the marketplace.

If the Primary DI has reached its lastShipDate, then any Package DI attached to the Primary DI will need to have a discontinuedDate populated. This ensures that a Package is not active and its contents are not.

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute cannot be deleted.



25. Package Status

FDA GUDID

Description	Indicates whether the package is in commercial distribution as defined under 21 CFR 807.3(b).
Data Entry Notes	Auto populated based on Package Discontinue Date. If Package DI and related elements are entered and no Package Distribution End Date is entered, the status is 'In Commercial Distribution.'
Edit Rules After Grace Period	NA (data element is not able to be changed directly; most are 'auto-populated' fields whose information depends on another data element)
Required?	Auto Populated
Data Type & Length	NA
Entry List of Values (LOV)	In Commercial Distribution; Not in Commercial Distribution
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Derived by the FDA GUDID based on effectiveDate and lastShipDate

Definition	N/A
Data Type	N/A
GDSN Required	N/A

Population Guidance (below)

If the current date is equal to or greater than the GUDID Publication Date (effectiveDate in GDSN) of the Primary DI, then the Package Status will be set to "In Commercial Distribution" automatically by the FDA. If the current date is equal to or greater than the GUDID Package Discontinue Date (lastShipDate for the package level GTIN in GDSN), then the Package Status will be set to "Not in Commercial Distribution" automatically by the FDA. Note, if the Commercial Distribution Status of the Primary DI is set to "Not in Commercial Distribution", the Package Status will also be set to "Not in Commercial Distribution".

26. Support Customer Contact Phone

FDA GUDID

Description	Phone number for the customer contact; to be used by patients and consumers for device-related questions.
Data Entry Notes	Enter phone number. For North American numbers, type 10-digit number with or without punctuation. For international numbers, start with "+" and type number without punctuation.
Edit Rules After Grace Period	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)
Required?	Conditionally Required* *ONLY required if Customer Contact Phone is entered
Data Type & Length	Type: Num. Length: 10 (North American numbers); 20 (all others)
Entry List of Values (LOV)	NA
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Attribute Name Pair of attributes in combination

- a. contactType
- b. communicationChannelCode
- c. communicationNumber

Definition

- a. The general category of the contact party for a trade item for example Purchasing.
- b. Means used to communicate with another party.
- c. Number assigned to a specific means of communication.

Data Type

- a. Code List
- b. Code List (Multiple Occurrence)
- c. Text (1-70 characters) (Multiple Occurrence)

GDSN Required- OPTIONAL, however if any of the three is provided, an instance of all three are required

Population Guidance (below)

The GDSN attribute contactType signifies which type of contact information is being provided. For end user or consumer support, the code value should be "CONSUMER\_SUPPORT". For the item's regulatory contact information, the code value should be "LICENSEE\_REGISTRAR". The GDSN attributes communicationChannelCode

and communicationNumber can repeat as a pair of attributes for a single contactType. There can be more than one contactType populated for a single Trade item.

For the GUDID, the contactType of "CONSUMER\_SUPPORT" will signify the information to be provided to the GUDID via GDSN. Where an instance of the GDSN attribute communicationChannelCode is populated with the value of "TELEPHONE", the corresponding communicationNumber will map to the GUDID attribute **Support-Customer** Contact Phone.

This group attributes will be used to provide several sets of information and as such will be repeated as a group. GUDID attributes using this group of attributes are **Support-Customer** Contact Phone and **Support-Customer** Contact Email.

27. **Support Customer Contact Email**

FDA GUDID

Description	Email for the Customer contact; to be used by patients and consumers for device-related questions.
Data Entry Notes	<p>Enter email address.</p> <p>This email address could be the same one that appears on the device labeling or the company website. Labelers can identify a Customer Contact email and a Customer Contact phone number for each device record.</p> <p>If a phone number is entered and you don't have a Customer Contact email, please enter 'xxx@xxx.xxx'</p>
Edit Rules After Grace Period	<p>Add (Addition of new data is allowed)</p> <p>Delete (Deletion of entered data is allowed)</p> <p>Edit (Editing of entered data is allowed)</p>
Required?	<p>Conditionally Required*</p> <p>*ONLY required if Customer Contact Email is entered</p>
Data Type & Length	<p>Type: Alphanum.</p> <p>Length: 100</p>
Entry List of Values (LOV)	NA
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Attribute Name- Pair of attributes in combination

- a. contactType
- b. communicationChannelCode
- c. communicationNumber

Definition

- a. The general category of the contact party for a trade item for example Purchasing.
- b. Means used to communicate with another party.
- c. Number assigned to a specific means of communication.

Data Type

- a. Code List
- b. Code List (Multiple Occurrence)
- c. Text (1-70 characters) (Multiple Occurrence)

GDSN Required- OPTIONAL, however if any of the three is provided, an instance of all three are required

Population Guidance (below)

The GDSN attribute contactType signifies which type of contact information is being provided. For end user or consumer support, the code value should be "CONSUMER\_SUPPORT". For the item's regulatory contact information, the code value

~~should be "LICENSEE\_REGISTRAR"~~. The GDSN attributes communicationChannelCode and communicationNumber can repeat as a pair of attributes for a single contactType. There can be more than one contactType populated for a single Trade item.

For the GUDID, the contactType of "CONSUMER\_SUPPORT" will signify the information to be provided to the GUDID via GDSN. Where an instance of the GDSN attribute communicationChannelCode is populated with the value of "EMAIL", the corresponding communicationNumber will map to the GUDID attribute ~~Support-Customer~~ Contact Email.

Where an instance of the GDSN attribute communicationChannelCode is populated with the value of "EMAIL", the corresponding communicationNumber will map to this GUDID attribute.

This group attributes will be used to provide several sets of information and as such will be repeated as a group. GUDID attributes using this group of attributes are ~~Support-Customer~~ Contact Phone and ~~Support-Customer~~ Contact Email.

28. Human Cell, Tissue or Cellular or Tissue-Based Product (HCT/P)

FDA GUDID

Description –	Indicates that the product contains or consists of human cells or tissues that are intended for implantation, transplantation, infusion, or transfer into a human recipient as defined under 21 CFR 1271.3.
Data Entry Notes	<p>Select checkbox if DI record is for a product defined under 21 CFR 1271.3</p> <p>If checked, the labeler must assign and label each HCT/P device with a distinct identification code, per 21 CFR 1271.290(c). The distinct identification code may take the form of a Donation Identification Number (DIN), serial number, lot number, or a combination of these production identifiers (PIs). Labelers of HCT/Ps regulated as medical devices should select the appropriate type of PI that appears on the label of the device.</p>
Edit Rules After Grace Period	<p>Add (Addition of new data is allowed)</p> <p>Delete (Deletion of entered data is allowed)</p> <p>Edit (Editing of entered data is allowed)</p>
Required?	<p>Optional</p> <p>If no data is provided, 'No' is stored</p>
Data Type & Length	Type: Boolean
Entry List of Values (LOV)	NA
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Attribute Name	doesTradeItemContainHumanTissue
Definition	The trade item has, as a component or ingredient, human tissue. The amount of tissue is not limited to a certain amount, any amount will cause a flag of “TRUE”.
Data Type	Boolean
GDSN Required	OPTIONAL

Population Guidance (below)

This Boolean attribute should be populated with a value of “TRUE” when there is any amount of human tissue as part of the device. Otherwise the value should default to FALSE.

29. Kit

FDA GUDID

Description –	Indicates that the device is a convenience, combination, in vitro diagnostic (IVD), or medical procedure kit. Kits are a collection of products, including medical devices, that are packaged together to achieve a common intended use and is being distributed as a medical device.
Data Entry Notes	Select checkbox if DI record is for a kit. Do not check if the device is a constituent part of a kit. (Webtool)
Edit Rules After Grace Period	None (NO edit, add, or delete are allowed)
Required?	Optional If no data is provided, 'No' is stored
Data Type & Length	Type: Boolean
Entry List of Values (LOV)	NA
New DI Trigger?	YES
Public/Private Status	Public

GS1 GDSN

Temporary population until final GDSN deployment

groupedProduct (value populated in GDSN is KIT)

Definition-	Code representing if the trade item is considered by the manufacturer to be more than a single item, such as a kit, combination item.
Data Type	Text
GDSN Required	Optional
Final Deployment Attribute Name	groupedProduct (value populated in GDSN is KIT)
Definition	Code representing if the trade item is considered by the manufacturer to be more than a single item, such as a kit, combination item.
Data Type	Code List
GDSN Required	OPTIONAL

Population Guidance (below)

This attribute has a temporary attribute (AVP) in GDSN- groupedProduct. It will be deployed into the GDSN Schema in 2016-17 into a final solution.

The GDSN attribute groupedProduct is a code list attribute. It is used to specify if an item is a kit or a combination product. A value populated for the GDSN attribute groupedProduct of "KIT" or "KIT AND COMBINATION" will populate a value of "TRUE" for the GUDID attribute Kit. Any other value, or when no value is provided, for the GDSN attribute will populate a value of "FALSE" for the GUDID attribute Kit.

This attribute will be used to provide several sets of information and as such may be repeated. GUDID attributes using this group-of attributes are Kit and Combination Products.

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can not be changed. Many of the data elements are locked and can no longer be edited.



### 30. Combination Product

#### FDA GUDID

Description –	Indicates that the product is comprised of two or more regulated products that are physically, chemically, or otherwise combined or mixed and produced as a single entity; packaged together as a single package; or packaged separately for the intended use together as defined under 21 CFR 3.2(e). At least one of the products in the combination product must be a device in this case.
Data Entry Notes	Check box if DI record is for the combination product itself. Do not check if the product is a constituent part of a combination product. (Webtool)
Edit Rules After Grace Period	None (NO edit, add, or delete are allowed)
Required?	Optional If no data is provided, 'No' is stored
Data Type & Length	Type: Boolean
Entry List of Values (LOV)	NA
New DI Trigger?	YES
Public/Private Status	Public

#### GS1 GDSN

Temporary population until final GDSN deployment

groupedProduct (value populated in GDSN is COMBINATION)

Definition-	Code representing if the trade item is considered by the manufacturer to be more than a single item, such as a kit, combination item.
Data Type	Text
GDSN Required	Optional
Final Deployment Attribute Name	groupedProduct (value populated in GDSN is COMBINATION)
Definition	Code representing if the trade item is considered by the manufacturer to be more than a single item, such as a kit, combination item.
Data Type	Code List
GDSN Required	OPTIONAL

#### Population Guidance (below)

This attribute has a temporary attribute (AVP) in GDSN- groupedProduct. It will be deployed into the GDSN Schema in 2016-17 into a final solution.

The GDSN attribute groupedProduct is a code list attribute. It is used to specify if an item is a kit or a combination product. A value populated for the GDSN attribute groupedProduct of "COMBINATION" or "KIT\_AND\_COMBINATION" will populate a value of "TRUE" for the GUDID attribute Combination Product. Any other value, or when no value is provided, for the GDSN attribute will populate a value of "FALSE" for the GUDID attribute Combination.

This attribute will be used to provide several sets of information and as such may be repeated. GUDID attributes using this **group of** attributes are Kit and Combination Products. Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can not be changed. Many of the data elements are locked and can no longer be edited.

31. Device Exempt from Premarket Authorization

FDA GUDID

Description	Device is exempt from FDA Premarket regulations; or a pre-amendment device.
Data Entry Notes	Select checkbox if FDA has by regulation exempted this device from premarket submission requirements; or for preamendment devices that are not subject to premarket submission requirements.  If left unselected, a 'No' is stored and a Premarket Submission Number should be entered below.
Edit Rules After Grace Period	None (NO edit, add, or delete are allowed)
Required?	Conditionally Required*  *Premarket Submission Number OR exempt status fulfills regulatory requirement.
Data Type & Length	Type: Boolean
Entry List of Values (LOV)	NA
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Temporary population until final GDSN deployment-  
exemptFromFDAPreMarketAuthorization

Definition- Device is exempt from FDA Premarket regulations. Premarket approval (PMA) is the FDA process of scientific and regulatory review to evaluate the safety and effectiveness of Class III medical devices. Class III devices are those that support or sustain human life, are of substantial importance in preventing impairment of human health, or which present a potential, unreasonable risk of illness or injury. Due to the level of risk associated with Class III devices, FDA has determined that general and special controls alone are insufficient to assure the safety and effectiveness of class III devices. Therefore, these devices require a premarket approval (PMA) application under section 515 of the FD&C Act in order to obtain marketing clearance. Please note that some Class III pre-amendment devices may require a Class III 510(k). See "Historical Background2" for additional information.

Data Type Text  
GDSN Required Optional  
Final Deployment Attribute Name-  
exemptFromFDAPreMarketAuthorization

Definition- Device is exempt from FDA Premarket regulations. Premarket approval (PMA) is the FDA process of scientific and regulatory review to evaluate the safety

and effectiveness of Class III medical devices. Class III devices are those that support or sustain human life, are of substantial importance in preventing impairment of human health, or which present a potential, unreasonable risk of illness or injury. Due to the level of risk associated with Class III devices, FDA has determined that general and special controls alone are insufficient to assure the safety and effectiveness of class III devices. Therefore, these devices require a premarket approval (PMA) application under section 515 of the FD&C Act in order to obtain marketing clearance. Please note that some Class III pre-amendment devices may require a Class III 510(k). See "Historical Background2" for additional information.

Data Type	BOOLEAN
GDSN Required	OPTIONAL

Population Guidance (below)

This attribute has a temporary attribute (AVP) in GDSN- exemptFromFDAPreMarketAuthorization. It will be deployed into the GDSN Schema in 2016-17 into a final solution.

This Boolean attribute is used to denote if an item is such that is does not require a pre-market authorization from the FDA (termed an exemption. A value of "TRUE" for this GDSN attribute signifies that the item has been deemed exempt from needing this type of review. A value of "FALSE" or a "NULL" value will signify that an authorization is required for the item.

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can not be changed. Many of the data elements are locked and can no longer be edited.

32. FDA Premarket Submission Number

FDA GUDID

Description –	Number associated with the regulatory decision regarding the applicant’s legal right to market a medical device for the following submission types: 510(k), PMA, PDP, HDE, BLA, and NDA.
Data Entry Notes	<p><b>Enter current FDA Premarket Submission Number(s).</b></p> <p><b>Each DI record represents a version or model of a device. For each DI record, you must submit the original premarket authorization number and the supplement number through which you obtained approval or clearance for the version or model identified in the DI record, as required by 830.310(b)(11). FDA Premarket Numbers should be verified with the FDA PMA or 510(k) database to make sure the Number represents the subject of the device record. Device records should be updated with additional numbers in the future, as needed.</b></p> <p><b>Example: PMA #123456 should be entered as 'P123456.'</b></p>
Edit Rules After Grace Period	<b>Add (Addition of new data is allowed)</b>
Required?	<b>Conditionally Required*</b>
	<b>*Premarket Submission Number OR exempt status fulfills regulatory requirement.</b>
Data Type & Length	<b>Type: Alphanumeric.</b> <b>Length: 8</b>
Entry List of Values (LOV)	<b>NA</b>
New DI Trigger?	<b>NO</b>
Public/Private Status	<b>Public</b>

GS1 GDSN

**Temporary population until final GDSN deployment**

**~~fDA510KPremarketAuthorization~~**

**Definition– Premarket approval (PMA) is the FDA process of scientific and regulatory review to evaluate the safety and effectiveness of Class III medical devices. These values are the 510K Premarket Authorization Numbers assigned to the item.**

**~~Data Type~~ ~~Text~~**

**~~GDSN Required~~ ~~Optional~~**

**~~Final Deployment Attribute Name~~**

Pair of attributes in combination

- a. additionalClassificationAgencyName (Code 58 for **"FDA\_510K\_PREMARKET\_NOTIFICATION"** **"FDA\_PREMARKET\_SUBMISSION\_NUMBER"**)
- b. additionalClassificationCategoryCode

Definition

- a. Text name of the additional external classification agency whose schema is being provided in addition to the Global EAN.UCC schema. Required if additional classification schema fields are populated.
- b. Category code based on alternate classification schema chosen in addition to EAN/UCC classification schema.

Data Type

- a. Code List (Multiple Occurrence)
- b. Text (1-35 characters) (Multiple Occurrence)

GDSN Required- OPTIONAL, however if one of the pair is populated the other must be populated.

Population Guidance (below)

~~This attribute has a temporary attribute (AVP) in GDSN- fda510KPreMarketAuthorization. It will be deployed into the GDSN Schema in 2016-17 into a final solution.~~

This set of attributes will allow for the population of a Pre-Market **Authorization Submission** Number for the device. This number will correlate to the scientific and regulatory review information which was created to evaluate the safety and efficacy of the device. This set of attributes is required to be provided when the value populated for the GDSN attribute `exemptFromFDAPreMarketAuthorization` is not "TRUE".

This set of attributes will also be used to populate several ~~other~~ pieces of information- FDA Product Code, FDA Premarket Submission Number, **FDA Preferred Term Code**, and GMDN. For supply chain use, this set of attributes can also provide the UNSPSC code for the device.

If there is a Supplement Number, place a colon (":") after the FDA Premarket Submission Number then add the Submission Number. Repeat these attributes and process for all applicable FDA Premarket Submission Numbers and Supplement Numbers.

For example, a device has a FDA Premarket Submission number of P369258. Over time 3 Supplements have been filed and approved 001, 002, and 004. Population of this information would look like this:

```

additionalClassificationAgencyName      58
additionalClassificationCategoryCode     P369258:001

additionalClassificationAgencyName      58
additionalClassificationCategoryCode     P369258:002

additionalClassificationAgencyName      58
additionalClassificationCategoryCode     P369258:004
    
```

For example, a device has a FDA Premarket Submission Number of P147025. Over time 2 Supplements have been filed and approved 001, 002. Then a second FDA Premarket Submission Number was obtained P963074 and a subsequent Supplement was filed and approved, 001. Population of this information would look like this:

```

additionalClassificationAgencyName      58
additionalClassificationCategoryCode     P147025:001

additionalClassificationAgencyName      58
additionalClassificationCategoryCode     P147025:002

additionalClassificationAgencyName      58
    
```

**additionalClassificationCategoryCode**      **P963074:001**

**The Data Pool will parse the supplement number from the FDA Premarket Submission Number and provide to the FDA GUDID in the two fields as required by the FDA.**

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can be added but can not be edited or deleted.

33. Supplement #

FDA GUDID

Description	Number assigned by FDA to a supplemental application for approval of a change in a medical device with an approved PMA, HDE, or PDP.
Data Entry Notes	<p>Enter all valid Supplement Numbers.</p> <p>Each DI record represents a version or model of a device. For each DI record, you must submit the original premarket authorization number and the supplement number through which you obtained approval for the version or model identified in that DI record, as required by 830.310(b)(11). Although not all PMA supplements are applicable to a given model or version, if FDA approves a subsequent supplement applicable to that version or model, the GUDID DI record must be updated with that supplement number, in accordance with 21 CFR 830.330(b). 30 day notice supplements should be submitted ONLY if the 30 day notice impacts the device design specifications, or performance of the finished devices.</p> <p>Do not enter alpha characters.</p> <p>Example: Supplement 4 should be entered as 004.</p>
Edit Rules After Grace Period Required?	<p>Add (Addition of new data is allowed)</p> <p>Conditionally Required*</p> <p>*Premarket Submission Number OR exempt status fulfills regulatory requirement.</p>
Data Type & Length	<p>Type: Num.</p> <p>Length: 4</p>
Entry List of Values (LOV)	NA
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

~~Temporary population until final GDSN deployment~~

~~\_\_\_\_\_fDASupplementNumber~~

~~Definition— Number associated with the regulatory decision regarding the applicant's legal right to market a medical device (PMA Supplement). After FDA has approved a PMA, an applicant must submit a PMA supplement for review and approval by FDA before making any change affecting the safety or effectiveness of the device unless FDA has advised that an alternate type of submission is permitted for a particular change. All changes must meet the requirements of the Quality System regulation (Good Manufacturing Practices) under 21 CFR Part 820 including the design control requirement under §820.30. Changes for which an applicant must submit a PMA supplement include, but are not limited to, the following types of changes if they affect the safety or effectiveness of the device: new indication for use of the device; labeling changes; the use of a different facility or establishment to manufacture, process, sterilize, or package the device; changes in manufacturing facilities, methods, or quality control procedures; changes in sterilization procedures; changes in~~



packaging; changes in the performance or design specifications, circuits, components, ingredients, principles of operation, or physical layout of the device; and extension of the expiration date of the device based on data obtained under a new or revised stability or sterility testing protocol that has not been approved by FDA. [If the protocol has been previously approved by FDA, a supplement is not submitted but the change must be reported to FDA in the post approval periodic reports as described in the §814.39(b).]

Data Type  Text

GDSN Required  Optional

Final Deployment Attribute Name `fDASupplementNumber`

Definition Number associated with the regulatory decision regarding the applicant's legal right to market a medical device (PMA Supplement). After FDA has approved a PMA, an applicant must submit a PMA supplement for review and approval by FDA before making any change affecting the safety or effectiveness of the device unless FDA has advised that an alternate type of submission is permitted for a particular change. All changes must meet the requirements of the Quality System regulation (Good Manufacturing Practices) under 21 CFR Part 820 including the design control requirement under §820.30. Changes for which an applicant must submit a PMA supplement include, but are not limited to, the following types of changes if they affect the safety or effectiveness of the device: new indication for use of the device; labeling changes; the use of a different facility or establishment to manufacture, process, sterilize, or package the device; changes in manufacturing facilities, methods, or quality control procedures; changes in sterilization procedures; changes in packaging; changes in the performance or design specifications, circuits, components, ingredients, principles of operation, or physical layout of the device; and extension of the expiration date of the device based on data obtained under a new or revised stability or sterility testing protocol that has not been approved by FDA. [If the protocol has been previously approved by FDA, a supplement is not submitted but the change must be reported to FDA in the post approval periodic reports as described in the §814.39(b).]

Data Type  Integer

GDSN Required  OPTIONAL

Definition- N/A

Data Type N/A

GDSN Required N/A

**Population Guidance**

This attribute has a temporary attribute (AVP) in GDSN `fDASupplementNumber`. It will be deployed into the GDSN Schema in 2016-17 into a final solution.

This is the FDA identification number associated to the regulatory decision regarding the applicant's legal right to market a medical device (PMA Supplement).

If there is a Supplement Number, place a colon (":") after the FDA Premarket Submission Number then add the Submission Number. Repeat these attributes and process for all applicable FDA Premarket Submission Numbers and Supplement Numbers.

For example, a device has a FDA Premarket Submission number of P369258. Over time 3 Supplements have been filed and approved 001, 002, and 004. Population of this information would look like this:

<code>additionalClassificationAgencyName</code>	58
<code>additionalClassificationCategoryCode</code>	P369258:001
<code>additionalClassificationAgencyName</code>	58

additionalClassificationCategoryCode	P369258:002
additionalClassificationAgencyName	58
additionalClassificationCategoryCode	P369258:004

For example, a device has a FDA Premarket Submission Number of P147025. Over time 2 Supplements have been filed and approved 001, 002. Then a second FDA Premarket Submission Number was obtained P963074 and a subsequent Supplement was filed and approved, 001. Population of this information would look like this:

additionalClassificationAgencyName	58
additionalClassificationCategoryCode	P147025:001
additionalClassificationAgencyName	58
additionalClassificationCategoryCode	P147025:002
additionalClassificationAgencyName	58
additionalClassificationCategoryCode	P963074:001

The Data Pool will parse the supplement number from the FDA Premarket Submission Number and provide to the FDA GUDID in the two fields as required by the FDA.

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can be added but can not be edited or deleted.

### 34. Product Code

#### FDA GUDID

Description	Classification for devices issued by the FDA.
Data Entry Notes	Enter all applicable Product Codes, three-letter code. For all PMA and 510k devices, Product Codes are assigned in the FDA approval or clearance letter, respectively. For Class I and exempt devices, the device Product Code may be self-identified.
Edit Rules After Grace Period	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)
Required	Conditionally Required* *Unless device is a kit or IVD with a BL premarket submission number
Data Type & Length	Type: Alpha Length: 3
Entry List of Values (LOV)	FDA Product Code list
New DI Trigger?	NO
Public/Private Status	Public

#### GS1 GDSN

Attribute Name	Pair of attributes in combination
a. additionalClassificationAgencyName	(Code 43 for "US FDA Product Code")
b. additionalClassificationCategoryCode	
Definition	
a.	Text name of the additional external classification agency whose schema is being provided in addition to the Global EAN.UCC schema. Required if additional classification schema fields are populated.
b.	Category code based on alternate classification schema chosen in addition to EAN/UCC classification schema.
Data Type	
a.	Code List (Multiple Occurrence)
b.	Text (1-35 characters) (Multiple Occurrence)
GDSN Required	OPTIONAL, however if one of the pair is populated the other must be populated.

#### Population Guidance (below)

This repeatable set of attributes will allow for the population of a FDA Product Code for the device. This can be accomplished by the population of the code value "43" in the GDSN attribute additionalClassificationAgencyName. The actual Product Code can then be populated using the associated value in the GDSN attribute additionalClassificationCategoryCode.

This set of attributes will also be used to populate several ~~other~~ pieces of information- FDA Product Code, FDA Premarket Submission Number, **FDA Preferred Term Code**, and GMDN. For supply chain use, this set of attributes can also provide the UNSPSC codes for the device.

35. Product Code Name

FDA GUDID

Description	Name associated with the three-letter Product Code.
Data Entry Notes	Auto populated based on 3-letter Product Code
Edit Rules After Grace Period	NA (data element is not able to be changed directly; most are 'auto-populated' fields whose information depends on another data element)
Required?	Auto Populated
Data Type & Length	NA
Entry List of Values (LOV)	NA
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Attribute Name	N/A
Definition	N/A
Data Type	N/A
GDSN Required	N/A

Population Guidance (below)

The FDA will automatically populate the GUDID with a value for this attribute based on the Product Code submitted.

36. FDA Listing Number

FDA GUDID

Description	Number assigned by FDA during Registration and Listing to all devices in commercial distribution, regardless of pre-market authorization requirements per 21 CFR 807.28(f).
Data Entry Notes	<p>Enter all relevant listing numbers that enable the labeler to commercially distribute the given version or model of device.</p> <p>Listing number is optional for HCT/P devices, Kits and IVDs with a BLA premarket number.</p>
Edit Rules After Grace Period	Add (Addition of new data is allowed)
Required?	Conditionally Required*
	*Unless device is an HCT/P, kit or IVD with a BLA premarket submission number
Data Type & Length	<p>Type: Alphanumeric.</p> <p>Length: 7</p>
Entry List of Values (LOV)	NA
New DI Trigger?	NO
Public/Private Status	Private

GS1 GDSN

Temporary population until final GDSN deployment-

fDAMedicalDeviceListing

Definition- Most Owners or operators of places of business (also called establishments or facilities) that are involved in the production and distribution of medical devices intended for use in the United States (U.S.) are required to list the devices that are made at their facility and the activities that are performed on those devices. Registration and listing provides FDA with the location of medical device establishments and the devices manufactured at those establishments. Knowing where devices are made increases the nation's ability to prepare for and respond to public health emergencies.

Data Type Text

GDSN Required Optional

Final Deployment Attribute Name Pair of attributes in combination

- a. additionalTradeItemIdentification\type (Code of "FDA\_MEDICAL\_DEVICE\_LISTING")
- b. additionalTradeItemIdentification\value

Definition

- a. Type of the identification system that is being used as an alternative to the Global Trade Item Number.
- b. Alternative means to the Global Trade Item Number to identify a trade item.

Data Type

- a. Code List (Multiple Occurrence)
- b. Text (Multiple Occurrence)

GDSN Required- OPTIONAL, however if one of the pair is populated the other must be populated.

Population Guidance (below)

This attribute has a temporary attribute (AVP) in GDSN- fdAMedicalDeviceListingNumber. It will be deployed into the GDSN Schema in 2016-17 into a final solution.

The GUDID is asking for the FPD Medical Device Listing number assigned to the device. This repeatable set of attributes will allow for the population of a FDA Medical Device Listing Number for the device. This can be accomplished by the population of the code value “FDA\_MEDICAL\_DEVICE\_LISTING” in the GDSN attribute additionalPartyIdentification/type. The actual FDA Medical Device Listing # can then populated in the GUDID using the associated additionalPartyIdentification\value(s).

This group attributes will be used to provide several sets of information and as such will be repeated as a group. GUDID attributes using this group of attributes are Version or Model Number, Catalog Number, Secondary DI Number, and FDA Listing Number.

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can be added but can not be edited or deleted.

37. Code SPL Name- GMDN Preferred Term Code and FDA Preferred Term Code

FDA GUDID

Description

GMDN Preferred Term (PT) Code is a unique five-digit code used to identify common device types. This PT Code is assigned to medical devices and related health care products for the purposes of grouping and categorization.

SPL Definition for GMDN Preferred Term (PT) Code: "Unique numerical five-digit number used to generically identify medical devices and related health care products."

SPL Definition for FDA Preferred Term Code: "Unique four-character value assigned by the FDA to indicate a GMDN Preferred Term without exposing the GMDN PT Code."

Data Entry Notes

Enter all applicable GMDN Preferred Term Codes or FDA PT Codes.

Each device record must have at least one assigned GMDN Code/FDA PT Code; DI records are allowed >1 GMDN Code/FDA PT Code, if necessary. Must enter GMDN Code OR FDA PT Code, please don't enter both codes for the same GMDN Name and Definition. The FDA PT Codes can be found in the Find FDA PT Code Module on the GUDID website.

For GMDN Codes: Enter only the 5-digit number, omit the 'P'

For FDA PT Codes: Enter the 4-letter code.

Edit Rules After Grace Period

Add (Addition of new data is allowed)

Delete (Deletion of entered data is allowed)

Edit (Editing of entered data is allowed)

Required?

Required, SPL Text: "Required - either GMDN PT Code or FDA PT Code"

Data Type & Length

Type: Num.

Length: 5,

SPL Text: "Alphanumeric, 5"

Entry List of Values (LOV)

NA

New DI Trigger?

NO

Public/Private Status

Private

GS1 GDSN

Attribute Name

Pair of attributes in combination

a. additionalClassificationAgencyName (Code of 35 for Global Medical Devices Nomenclature (GMDN))

b. additionalClassificationCategoryCode

Definition



- a. Text name of the additional external classification agency whose schema is being provided in addition to the Global EAN.UCC schema. Required if additional classification schema fields are populated.
- b. Category code based on alternate classification schema chosen in addition to EAN/UCC classification schema.

Data Type

- a. Code List (Multiple Occurrence)
- b. Text (1-35 characters) (Multiple Occurrence)

GDSN Required

OPTIONAL, however if one of the pair is populated the other must be populated.

Population Guidance (below)

This repeatable set of attributes will allow for the population of a **FDA Product Code GMDN Code** for the device. This can be accomplished by the population of the code value "35" in the GDSN attribute `additionalClassificationAgencyName`. The actual GMDN Code can then be populated using the associated value in the GDSN attribute `additionalClassificationCategoryCode`. Only the GMDN **Code Preferred Term** will be populated in the GUDID.

This set of attributes will also be used to populate several **other** pieces of information- FDA Product Code, FDA Premarket Submission Number, **FDA Preferred Term Code**, and GMDN. For supply chain use, this set of attributes can also provide the UNSPSC codes for the device.

*The SPL Guidance states "As stipulated in the Final UDI Rule [78 FR 58786], FDA has developed a new GUDID module, Find FDA Preferred Term (PT) Codes, that will enable users to select a FDA PT Code to be used in their GUDID submission until a GMDN PT code can be obtained from the GMDN Agency. The Find FDA PT Code module is enabled in GUDID v1.1 and can be accessed via the GUDID Web Interface by Coordinator and Labeler Data Entry (LDE) Users of GUDID. Note: these FDA PT Codes only apply to GUDID cannot be used in place of GMDN PT Codes for any other system."*

The population of a GMDN Code via GDSN has been available for some time. While the FDA will not make the code available to the Public in the GUDID, GDSN will pass the code along to normal GDSN recipients for their use following their existing processes. **The FDA will use the code provided to access the GMDN Preferred Term from the current GMDN Codeset. While the GMDN Code will not be published on the FDA GUDID Portal, the applicable GMDN Preferred Term will be published.**

38. Name

FDA GUDID

Description	Name associated with the GMDN Preferred Term Code /FDA PT Code.
Data Entry Notes	System populated based on GMDN Preferred Term Code/FDA PT Code.
Edit Rules After Grace Period	NA (data element is not able to be changed directly; most are 'auto-populated' fields whose information depends on another data element)
Required?	Auto Populated
Data Type & Length	NA
Entry List of Values (LOV)	NA
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Attribute Name	additionalClassificationCategoryDescription
Definition	In the additional classification system, the description of the category.
Data Type	Text (1-70 characters)
GDSN Required	Optional

Population Guidance (below)

The FDA will automatically populate the GUDID with a value for this attribute based on the GMDN Preferred Term Code (GMDN) submitted. Publishing the description field with the classification code name or description will provide additional value to supply chain partners receiving the message.

The population of a GMDN Code via GDSN has been available for some time. While the FDA will not make the code available to the Public in the GUDID, GDSN will pass the code along to normal GDSN recipients for their use following their existing processes.

39. Definition

FDA GUDID

Description	Description associated with the GMDN Preferred Term Code/ <b>FDA PT Code</b> ..
Data Entry Notes	System populated based on GMDN Preferred Term Code/ <b>FDA PT Code</b> ..
Edit Rules After Grace Period	<b>NA (data element is not able to be changed directly; most are 'auto-populated' fields whose information depends on another data element)</b>
Required?	<b>Auto Populated</b>
Data Type & Length	<b>NA</b>
Entry List of Values (LOV)	<b>NA</b>
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Attribute Name	N/A
Definition	N/A
Data Type	N/A
GDSN Required	1..1, Required

Population Guidance (below)

The FDA will automatically populate the GUDID with a value for this attribute based on the **GMDN Preferred Term** Code ~~(GMDN)~~ submitted.

#### 40. For Single Use

##### FDA GUDID

Description	Indicates that the device is intended for one use or on a single patient during a single procedure.
Data Entry Notes	Choose <b>Yes/No</b> from the drop down <b>list</b> . (Webtool)
Edit Rules After Grace Period	<b>None (NO edit, add, or delete are allowed)</b>
Required?	<b>Required</b>
Data Type & Length	<b>Type: Boolean</b>
Entry List of Values (LOV)	Yes/No
New DI Trigger?	YES
Public/Private Status	Public

##### GS1 GDSN

Attribute Name	manufacturerDeclaredReusabilityType
Definition-	Determines if the product is intended for single or multiple uses; including the number of validated cycles and the number of times a product can be used according to the manufacturer specifications. It is suggested that medical providers consult the device manufacturer's Instruction For Use (IFU) for full reusability instructions.
Data Type	Code List
GDSN Required	OPTIONAL

##### Population Guidance (below)

This **GDSN** attribute is a code list stating if the item can be used again. When a value of "SINGLE\_USE" or "REUSABLE\_SAME\_PATIENT" are populated for the GDSN attribute manufacturerDeclaredReusabilityType, the GUDID will be populated with a value of "TRUE" signifying the device is intended for one use or **multiple uses** on a single **patient**. For all other values populated in the GDSN attribute manufacturerDeclaredReusabilityType, the GUDID will be populated with a value of "FALSE" signifying the device can be used more than one time **on multiple patients**.

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can not be changed. Many of the data elements are locked and can no longer be edited.

41. Lot or Batch Number

FDA GUDID

Description –	Indicates the device is managed by lot or batch number. This number can be found on the device label or packaging. Lot or Batch means one finished device or more that consist of a single type, model, class, size, composition, or software version that are manufactured under essentially the same conditions and that are intended to have uniform characteristics and quality within specified limits.
Data Entry Notes	Choose Yes/No from the drop down list.  For stand-alone software, select Yes to indicate that the software version number will be represented as a Lot or Batch number
Edit Rules After Grace Period	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)
Required?	Required
Data Type & Length	Type: Boolean
Entry List of Values (LOV)	Yes/No
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Attribute Name	hasBatchNumber
Definition-	Indication whether the base trade item is batch or lot number requested by law, not batch or lot number requested by law but batch or lot number allocated, or not batch or lot number allocated. A batch or lot number is a manufacturer assigned code used to identify a trade items trade item on batch or lot. Differs from Serial Number, which is a manufacturer assigned code during the trade item on cycle to identify a unique trade item.
Data Type	Boolean
GDSN Required	OPTIONAL

Population Guidance (below)

This attribute is a Boolean clarifying how the item is controlled. It is not for the population of actual lot or batch numbers. Neither the GUDID nor GDSN are used to provide actual Batch or Lot numbers. These should be communicated in transactional documents such as packaging, shipping and invoice documents.

A value populated of “TRUE” signifies that the device has, as one of its controls, a batch or lot number. It also signifies that the batch or lot number will be printed on the packaging and in the UDI.

#### 42. Manufacture Date

##### FDA GUDID

Description	Indicates the device is managed by date of manufacture; the date a specific device was manufactured.
Data Entry Notes	Choose Yes/No from the drop down list. (Webtool)
Edit Rules After Grace Period	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)
Required?	Required
Data Type & Length	Type: Boolean
Entry List of Values (LOV)	Yes/No
New DI Trigger?	NO
Public/Private Status	Public

##### GS1 GDSN

Temporary population until final GDSN deployment-

isTradelItemManagedByManufactureDate

Definition- Indication whether the trade item is managed by manufacture date. A positive response indicates the manufacturer utilizes the manufacture date to control the item instead of lot and batch numbers.

Data Type Boolean

GDSN Required Optional

Final Deployment Attribute Name

tradelItemDateOnPackagingTypeCode (coming in Major Release in 2016)

Definition Indicates the type of date marked on the packaging for example Best Before Date.

Data Type Code List

GDSN Required OPTIONAL

##### Population Guidance (below)

This attribute has a temporary attribute (AVP) in GDSN

isTradelItemManagedByManufactureDate.

It will be deployed into the GDSN Schema in 2016 into a final solution.

This GUDID attribute is a Boolean clarifying how the item is controlled. It is not for the population of actual manufacturing dates. Neither the GUDID nor GDSN are used to provide actual manufacturing dates. These should be communicated in transactional documents such as packaging, shipping and invoice documents.

A value populated of "TRUE" for the temporary attribute or of "PRODUCTION\_DATE" for the attribute tradelItemDateOnPackagingTypeCode signifies that the item has, as one of its controls, a manufacture date. It also signifies that the manufacture date will be printed on the packaging and in the UDI.

### 43. Serial Number

#### FDA GUDID

Description –	Indicates the device is managed by serial number. This number can be found on the device label or packaging. The serial number is assigned by the labeler and should be specific to each device.
Data Entry Notes	Choose Yes/No from the drop down list. (Webtool)
Edit Rules After Grace Period	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)
Required?	Required
Data Type & Length	Type: Boolean
Entry List of Values (LOV)	Yes/No
New DI Trigger?	NO
Public/Private Status	Public

#### GS1 GDSN

Attribute Name	serialNumberLocationCode
Definition-	The location on the item or packaging of a serial number. A serial number is a code, numeric or alphanumeric, assigned to an individual instance of an entity for its lifetime for example a Microscope model AC-2 with serial number 1234568 and microscope model AC-2 with serial number 1234569.
Data Type	Text (1-35 characters) (External Code List)
GDSN Required	OPTIONAL

#### Population Guidance (below)

This GUDID attribute is a Boolean clarifying how the item is controlled. It is not for the population of an actual serial number(s). Neither the GUDID nor GDSN are used to provide an actual serial numbers(s). These should be communicated in transactional documents such as packaging, shipping and invoice documents.

A GUDID value of “TRUE” signifies that the item has, as one of its controls, a serial number(s). It also signifies that the manufacture date will be printed on the packaging and in the UDI.

This GDSN attribute is a code list attribute designating where the serial number can be found on the item or its packaging, if present. If a value is populated for the GDSN attribute of “MARKED\_ON\_PACKAGING”, “MARKED\_ON\_PACKAGING\_INSERT”, or “MARKED\_ON\_TRADE\_ITEM”, it signifies that the item has, as one of its controls, a serial number and a value of “TRUE” will be populated for the GUDID attribute. It also signifies that the serial number will be printed on the packaging and in the UDI. Any other code value published in GDSN will populate a value of “FALSE” for the GUDID attribute.

#### 44. By Expiration Date

##### FDA GUDID

Description	Indicates the device is managed by expiration date; the date by which the label of a device states that the device must or should be used.
Data Entry Notes	Choose Yes/No from the drop down list. (Webtool)
Edit Rules After Grace Period	Add (Addition of new data is allowed)
	Delete (Deletion of entered data is allowed)
	Edit (Editing of entered data is allowed)
Required?	Required
Data Type & Length	Type: Boolean
Entry List of Values (LOV)	Yes/No
New DI Trigger?	NO
Public/Private Status	Public

##### GS1 GDSN

Current GDSN Attribute	packagingMarkedExpirationDateType
Definition	Indicates the type of expiration date marked on the packaging for example Best Before Date.
Data Type	Code List
GDSN Required	OPTIONAL
Final Deployment Attribute Name-	
	tradeltemDateOnPackagingTypeCode (coming in Major Release in 2016)
Definition	Indicates the type of date marked on the packaging for example Best Before Date.
Data Type	Code List
GDSN Required	OPTIONAL

##### Population Guidance (below)

This attribute has a current attribute in GDSN- packagingMarkedExpirationDateType. It will be changed in the GDSN Major Release in 2016 into the attribute tradeltemDateOnPackagingTypeCode.

This GUDID attribute is a Boolean clarifying how the item is controlled. It is not for the population of actual expiration dates. Neither the GUDID nor GDSN are used to provide actual expiration dates. These should be communicated in transactional documents such as packaging, shipping and invoice documents.

A value populated of "BEST\_BEFORE\_DATE" or "EXPIRY\_DATE" for the current GDSN attribute packagingMarkedExpirationDateType or of "BEST\_BEFORE\_DATE" or "EXPIRATION\_DATE" for the attribute tradeltemDateOnPackagingTypeCode signifies that the item has, as one of its controls, an expiration date. These values signifies that the expiration date will be printed on the packaging and in the UDI. A value of "TRUE" will be populated in the GUDID for these codes. Any other code for these GDSN Attributes will populate a value of "FALSE" for the GUDID.



**45. Donation Identification Number**

**FDA GUDID**

Description –	SPL Definition: "Indicates the device is managed by a Donation Identification Number. This number can be found on the device label or packaging. The Donation Identification Number is applicable to devices that are also regulated as HCT/Ps and is a number that is assigned to each donation."
Data Entry Notes	Choose Yes/No from the drop down list. This PI is only applicable to HCT/P products regulated as medical devices.
Edit Rules After Grace Period	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)
Required?	Required
Data Type & Length	Type: Boolean
Entry List of Values (LOV)	Yes/No
New DI Trigger?	YES
Public/Private Status	Public

**GS1 GDSN**

Temporary population until final GDSN deployment-  
donationIdentificationNumberMarked

Definition-	Indicates the device is managed by a Donation Identification Number. This number can be found on the device label or packaging. The Donation Identification Number is applicable to devices that are also regulated as HCT/Ps and is a number that is assigned to each donation.
Data Type	Boolean
GDSN Required	Optional

**Final Deployment Attribute Name**

donationIdentificationNumberMarked (coming in a future GDSN Release about 2016-17)

Definition	Indicates the device is managed by a Donation Identification Number. This number can be found on the device label or packaging. The Donation Identification Number is applicable to devices that are also regulated as HCT/Ps and is a number that is assigned to each donation.
Data Type	Boolean
GDSN Required	OPTIONAL

**Population Guidance (below)**

This attribute has a temporary attribute (AVP) in GDSN-  
donationIdentificationNumberMarked. It will be deployed into the GDSN Schema in 2016-17  
into a final solution.

This GUDID attribute is a Boolean clarifying how the item is controlled. It is not for the  
population of actual Donation Identification Numbers. Neither the GUDID nor GDSN are  
used to provide actual Donation Identification Numbers. These should be communicated in  
transactional documents such as packaging, shipping and invoice documents.

46. Device required to be labeled as containing natural rubber latex or dry natural rubber (21 CFR 801.437)

FDA GUDID

Description –	Indicates that the device or packaging contains natural rubber that contacts humans as described under 21 CFR 801.437. Choosing 'Yes' indicates that the device label or packaging contains one of the following statements: (1) "Caution: This Product Contains Natural Rubber Latex Which May Cause Allergic Reactions", (2) This Product Contains Dry Natural Rubber", (3) Caution: The Packaging of This Product Contains Natural Rubber Latex Which May Cause Allergic Reactions" or (4) "The Packaging of This Product Contains Dry Natural Rubber".
Data Entry Notes	Choose Yes/No from the drop down list. (Webtool)
Edit Rules After Grace Period	None (NO edit, add, or delete are allowed)
Required?	Required
Data Type & Length	Type: Boolean
Entry List of Values (LOV)	Yes/No
New DI Trigger?	YES
Public/Private Status	Public

GS1 GDSN

Attribute Name	doesTradeltemContainLatex
Definition-	An indication that a trade item is made from or contains latex which refers generically to a stable dispersion (emulsion) of polymer microparticles in an aqueous medium.
Data Type	Non-Binary Logic
GDSN Required	OPTIONAL

Population Guidance (below)

This GDSN attribute is a Non-Binary Logic Code List with the values of "TRUE", "FALSE", "NOT\_APPLICABLE", and "UNSPECIFIED". For the US Target Market, the only values, which can be used are "TRUE" and "FALSE" for medical devices. All other values should not be accepted for a GDSN Target Market value of 840 (US).

Application of the value is based upon whether a mark exists on the packaging as to latex being contained in the device or its packaging. If a mark is required to be on the package, this attribute is populated with "TRUE". If no mark is required, then this attribute is populated with "FALSE". This is based on the regulation, which basically states that if there is latex present a label mark must be placed on the packaging.

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can not be changed. Many of the data elements are locked and can no longer be edited.

47. Device labeled as "Not made with natural rubber latex"

FDA GUDID

Description	"Indicates that natural rubber latex was not used as materials in the manufacture of the medical product and container and the device labeling contains this information. Only applicable to devices not subject to the requirements under 21 CFR 801.437. Not all medical products that are NOT made with natural rubber latex will be marked.
Data Entry Notes	<p>Select checkbox if appropriate.</p> <p>Only applicable if the response to "Device required to be labeled as containing natural rubber latex or dry natural rubber" is "No".</p> <p>Optional element for labelers who include a statement of 'latex-free' on their label or in their labeling. FDA finds these statements: 'latex-free' and 'does not contain latex', to be not scientifically supportable and strongly recommends they not be used in medical product labeling. Instead FDA recommends the use of the statement 'Not made with natural rubber latex.'</p> <p>It is not assumed that all devices NOT made with natural rubber latex are marked; therefore this is an optional element for the labelers who choose to make a statement in the labeling.</p>
Edit Rules After Grace Period –	<p>Add (Addition of new data is allowed)</p> <p>Delete (Deletion of entered data is allowed)</p> <p>Edit (Editing of entered data is allowed)</p>
Required?	<p>Optional</p> <p>If no data is provided, "No" is stored</p>
Data Type & Length	Type: Boolean
Entry List of Values (LOV)	NA
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Attribute Name	packageMarksFreeFrom
Definition	Indication of the food ingredients that the package is marked free from.
Data Type	Code List
GDSN Required	OPTIONAL

Population Guidance (below)

This GDSN attribute is a code list of values representing markings on the packaging. The markings signify the device is "Free-from" certain ingredients (irritants or allergens). This GDSN attribute is only populated to signify what is called out in one of these markings. The device might be free from one or more of the ingredients signified by a code value in the

code list. However, the actual code value is only populated here if there is an actual mark on the package calling out the ingredient is not present.

If a value of "FREE\_FROM\_LATEX" is published in the GDSN attribute packageMarksFreeFrom attribute, a value of "TRUE" will be populated in the GUDID. Any other code value published in GDSN will populate a value of "FALSE" for this GUDID attribute.

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can be edited, but only under certain circumstances. See Edit Rules After Grace Period for more details

48. Prescription Use (Rx)

FDA GUDID

Description	Indicates that the device requires a prescription to use.
Data Entry Notes	Select checkbox if appropriate. Can select both Rx and OTC for one DI record. (Webtool)
Edit Rules After Grace Period	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)
Required?	Optional If no data is provided, "No" is stored
Data Type & Length	Type: Boolean
Entry List of Values (LOV)	NA
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Attribute Name	ConsumerSalesCondition
Definition	A code depicting restrictions imposed on the Trade Item regarding how it can be sold to the consumer for example Prescription Required.
Data Type	Code List
GDSN Required	OPTIONAL

Population Guidance (below)

This GDSN attribute is a code list of values signifying how the item is presented for sale to a consumer.

If a value of "PRESCRIPTION\_REQUIRED" is published in the GDSN attribute ConsumerSalesCondition attribute, a value of "TRUE" will be populate in the GUDID. Any other code value published in GDSN will populate a value of "FALSE" for this GUDID attribute.

49. Over the Counter (OTC)

FDA GUDID

Description	Indicates that the device does not require a prescription to use and can be purchased over the counter (OTC).
Data Entry Notes	Select checkbox if appropriate. Can select both Rx and OTC for one DI record. (Webtool)
Edit Rules After Grace Period	Add (Addition of new data is allowed) Delete (Deletion of entered data is allowed) Edit (Editing of entered data is allowed)
Required?	Optional If no data is provided, "No" is stored
Data Type & Length	Type: Boolean
Entry List of Values (LOV)	NA
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Attribute Name	ConsumerSalesCondition
Definition	A code depicting restrictions imposed on the Trade Item regarding how it can be sold to the consumer for example Prescription Required.
Data Type	Code List
GDSN Required	OPTIONAL

Population Guidance (below)

This GDSN attribute is a code list of values signifying how the item is presented for sale to a consumer.

If a value of "OTC" is published in the GDSN attribute ConsumerSalesCondition attribute, a value of "TRUE" will be populate in the GUDID. Any other code value published in GDSN will populate a value of "FALSE" for this GUDID attribute.

**50. Is the device labeled for MRI Safety?—Removed this attribute as of 5/7/2014**

**FDA GUDID**

**Description** ————— Indicates that sufficient testing has been conducted to characterize the behavior of the device in the MR environment. See ASTM F2503-13.

**Data Entry Notes** ————— Check box if appropriate. (Webtool)

**Edit Rules After Grace Period** ————— Can add check to checkbox after Grace Period, but cannot delete a check from the checkbox.

**Required?** ————— 0..1 Not Required

**Data Type & Length** ————— Boolean

**Entry List of Values (LOV)** ————— Yes/No

**New DI Trigger?** ————— NO

**Public/Private Status** ————— Public

**GS1 GDSN**

**Attribute Name** ————— N/A- LOGICAL POPUALTION

**Definition** ————— N/A

**Data Type** ————— N/A

**GDSN Required** ————— N/A

**Population Guidance (below)**

**LOGICAL POPULATION**—On the outbound GUDID Message by the Data Pool. Will use the value "TRUE" when any code value other than "UNSPECIFIED" or "MRI\_UNSAFE" is published in the GDSN attribute mRICompatibility. By using GDSN, the GTIN of the lowest level of the hierarchy will become the Primary DI.

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can only be changed to a value of "TRUE" from a value of "FALSE". If the value needs to be changed to a value of "FALSE" from a value of "TRUE", a new UDI will be required.

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can be added but can not be deleted.



51. **MRI Safety Status** What MRI safety information does the labeling contain?

FDA GUDID

Description –	Indicates the MRI Safety Information, if any, that is present in the device labeling. Please see the ASTM F2503-13 standard for more information.
Data Entry Notes	Choose a value from the drop down LOV.  The final rule does not require MRI-compatibility testing; it only requires submission of information regarding MRI-compatibility that the labeler already possesses. (Webtool)
Edit Rules After Grace Period –	Choose a value from the drop down LOV.  The final rule does not require MRI-compatibility testing; it only requires submission of information regarding MRI-compatibility that the labeler already possesses.
Required?	Required
Data Type & Length	NA
Entry List of Values (LOV)	MR Safe, MR Unsafe, MR Conditional, Labeling does not contain MRI Safety information
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Attribute Name	mRICompatibility
Definition	This is an identification of the compatibility of a trade item for use in the presence of a Magnetic Resonance Imaging (MRI) system.
Data Type	Code List
GDSN Required	OPTIONAL

Population Guidance (below)

This GDSN attribute is a code list of values signifying if the device is safe for use in an MRI environment.

All GDSN code values map to an applicable GUDID code value. While it is not recommended to use a GDSN value of UNSPECIFIED as this provides no useful information and can lead to confusion in a clinical setting. However, if a GDSN value of UNSPECIFIED is published, this will be mapped to MR Unsafe as a default

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can be edited, but only under certain circumstances. See Edit Rules After Grace Period for more details

52. Size Type

FDA GUDID

Description Dimension type for the clinically relevant measurement of the medical device.

Data Entry Notes **Choose a value from the drop down LOV.**  
**If the desired Size Type is not in the current list, select 'Size Text, specify' and the data element 'Size Type Text' will appear (see below). It is expected that the 'Size Text, specify' will only be available for a limited time. Use this option to help us build a list of values that are appropriate for your device type. GUDID reserves the right to review all suggestions before adding values to the Size Type LOV.**

**More than one Size Value per Type and more than one Size Type may be added to each DI record.**

Edit Rules After Grace Period **Add (Addition of new data is allowed)**

Required? **Conditionally Required\***

**\*If device is available in more than one size**

Data Type & Length **NA**

Entry List of Values (LOV) – **CV – see vocab list Circumference; Depth; Device Size Text, specify; French Catheter Gauge; Greatest Diameter; Height; Length; Lumen Diameter; Needle Gauge; Second Greatest Diameter; Third Greatest Diameter; Total Volume; Width**

New DI Trigger? **NO**

Public/Private Status **Public**

GS1 GDSN

Temporary population until final GDSN deployment

clinicalSizeType

Definition The qualifier to denote the dimensional size which is clinically relevant for the use of the trade item by the clinical user. For example "needle gauge" for a 16 gauge needle, or "volume" for a 200 cc syringe.

Data Type Code List

GDSN Required OPTIONAL

Final Deployment Attribute Name clinicalSizeType

Definition The qualifier to denote the dimensional size which is clinically relevant for the use of the trade item by the clinical user. For example "needle gauge" for a 16 gauge needle, or "volume" for a 200 cc syringe.

Data Type Code List

GDSN Required OPTIONAL

Population Guidance (below)

This attribute has a temporary attribute (AVP) in GDSN- clinicalSizeText. It will be deployed into the GDSN Schema in 2016-17 into a final solution.

All of the clinical attributes can be repeated as a group when this value changes.

This GUDID attribute is a Code List clarifying the qualifier (type) associated to the clinical size values. For example as syringe is measured by the gauge of the needle and/or the volume it can contain. For the type, this attribute might be populated with "NEEDLE\_GAUGE" and/or "TOTAL\_VOLUME". This attribute is part of a repeatable class of clinical attributes for the device containing the Size Type, Size Value and Size Unit of Measure for the device's clinical size.

There is an option to specify a textual value for a clinical size type, which has not been specified in the value and UoM attributes.

When this attribute is published with the value of "DEVICE\_SIZE\_TEXT,\_SPECIFY", the GDSN attribute clinicalSizeText becomes required.

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can be added but can not be edited or deleted.

53. Size Value

FDA GUDID

Description	Numeric value for the clinically relevant size measurement of the medical device.
Data Entry Notes	<b>Enter numeric value for size.</b> <b>Decimals are accepted; fractions are not accepted. Each Size Value should be entered separately. GUDID is not accepting Size Value as a range at this time.</b>
Edit Rules After Grace Period	<b>Add (Addition of new data is allowed)</b>
Required?	<b>Conditionally Required*</b> <b>*Required if device is available in more than one size</b>
Data Type & Length	<b>Type: Num.</b> <b>Length: 40</b>
Entry List of Values (LOV)	<b>NA</b>
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Temporary population until final GDSN deployment-  
clinicalSizeValue

Definition	The value to denote the dimensional size which is clinically relevant for the use of the trade item by the clinical user. For example 16 gauge for a needle, or 200 cc for a syringe. Carries a UoM from the Recommendation 20 code list.
Data Type	Numeric
GDSN Required	OPTIONAL

Final Deployment Attribute Name clinicalSizeValue

Definition- The value to denote the dimensional size, which is clinically relevant for the use of the trade item by the clinical user. For example 16 gauge for a needle, or 200 cc for a syringe. Carries a UoM from the Recommendation 20 code list.

Data Type	Measurement (numeric & UoM qualifier)
GDSN Required	OPTIONAL

Population Guidance (below)

This attribute has a temporary attribute (AVP) in GDSN- clinicalSizeValue. It will be deployed into the GDSN Schema in 2016-17 into a final solution.

This GUDID attribute is a measurement attribute specifying the clinical measure of the device. This attribute is a numeric value and an associated Unit of Measure (UoM) qualifier. The UoM is a code from the UN Recommendation 20 Code List. The Data Pools will convert the UN Rec 20 code to the applicable code for the GUDID if needed. For the GUDID, the

data pools will populate the numeric value in the GUDID attribute Size Value and the UoM qualifier in the GUDID attribute Size Unit of Measure.

For example, for a 16 gauge needle the value is 16 and the UoM is H79, for a 20 cc syringe the value is 20 and the UoM is CQM

This attribute is part of a repeatable class of clinical attributes for the device containing the Size Type, Size Value and Size Unit of Measure for the device's clinical size.

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can be added but can not be edited or deleted.

54. Size Unit of Measure

FDA GUDID

Description	<p>The unit of measure associated with each clinically relevant size.</p> <p>SPL Text: "The unit of measure associated with each clinically relevant size. The unit of measure must conform to UCUM standards."</p>
Data Entry Notes	Choose a value from the drop down. (Webtool)
Edit Rules After Grace Period	Add (Addition of new data is allowed)
Required?	Conditionally Required*
	*Required if device is available in more than one size
Data Type & Length	NA
Entry List of Values (LOV)	<p>For length: Centimeter; Decimeter; Feet; Femtometer; Inch; Kilometer; Meter; Micrometer; Millimeter; Nanometer; Picometer; Yard;</p> <p>For area: Square centimeter; Square foot; Square inch; Square meter; Square millimeter</p> <p>For weight: Gram; Kilogram; Microgram; Milligram; Metric Ton; Pound; Ton</p> <p>For total volume: Centiliter; Cubic Inch; Cup; Deciliter; Femtoliter; Fluid Ounce; Gallon; Kiloliter; Liter; Microliter; Milliliter; Nanoliter; Picoliter; Pint; Quart</p> <p>For gauge: French; Gauge</p> <p>For angle: Degree</p> <p>For pressure: Pound per Square Inch; millibar; KiloPascal; Microgram per Total Volume; Milligram per Total Volume; Units per Liter; Hertz;</p> <p>SPL Text: "UCUM list of allowable values"</p>
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Temporary population until final GDSN deployment-  
clinicalSizeUoM

Definition-	The value to denote the dimensional size which is clinically relevant for the use of the trade item by the clinical user. For example 16 gauge for a needle, or 200 cc for a syringe. Carries a UoM from the Recommendation 20 code list.
Data Type	Code List (UoM qualifier)
GDSN Required	OPTIONAL
Final Deployment Attribute Name	clinicalSizeValue

Definition – The value to denote the dimensional size which is clinically relevant for the use of the trade item by the clinical user. For example 16 gauge for a needle, or 200 cc for a syringe. Carries a UoM from the Recommendation 20 code list.

Data Type Measurement (numeric & UoM qualifier)

GDSN Required OPTIONAL

Population Guidance (below)

This attribute has a temporary attribute (AVP) in GDSN- clinicalSizeValueUoM. It will be deployed into the GDSN Schema in 2016-17 into a final solution.

This GUDID attribute is a code list attribute specifying the clinical size unit of measure for the device's clinical size value. This attribute is a numeric value and an associated Unit of Measure (UoM) qualifier. The UoM is a code from the UN Recommendation 20 Code List. The Data Pools will convert the UN Rec 20 code to the applicable code for the GUDID if needed. For the GUDID, the data pools will populate the numeric value in the GUDID attribute Value and the UoM qualifier in the GUDID attribute Unit of Measure.

For example, for a 16 gauge needle the value is 16 and the UoM is H79, for a 20 cc syringe the value is 20 and the UoM is CQM

This attribute is part of a repeatable class of clinical attributes for the device containing the Size Type, Size Value and Size Unit of Measure for the device's clinical size.

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can be added but can not be edited or deleted.

55. Size Type Text **SPL Name: "Size Text"**

FDA GUDID

Description	Additional undefined device size not represented in the GUDID Size Type LOV.
Data Entry Notes	Enter Size Type, Size Unit and Unit of Measure for each entry.
Edit Rules After Grace Period	Add (Addition of new data is allowed)
Required?	Conditionally Required* *Required if 'Size Text, specify' is selected above
Data Type & Length	Type: Alphanum. Length: 200
Entry List of Values (LOV)	NA
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Temporary population until final GDSN deployment-  
clinicalSizeText

Definition	When the clinicalSizeType is coded as "other", this is the text used to denote the dimensional size which is clinically relevant for the use of the trade item by the clinical user.
Data Type	Text (1-200 characters)
GDSN Required	OPTIONAL
Final Deployment Attribute Name	clinicalSizeText
Definition	When the clinicalSizeType is coded as "other", this is the text used to denote the dimensional size which is clinically relevant for the use of the trade item by the clinical user.
Data Type	Text (1-200 characters)
GDSN Required	OPTIONAL

Population Guidance (below)

This attribute provides a value for this attribute when the GDSN attribute clinicalSizeType is required to be populated when a value of "OTHER" or "DEVICE\_SIZE\_TEXT,\_SPECIFY" is published in the GDSN attribute clinicalSizeType. This is free text field and should only be used if the clinical size can not be specified using specific values in the Clinical Size Type Code List.

This attribute is part of a repeatable class of clinical attributes for the device containing the Size Type, Size Value and Size Unit of Measure for the device's clinical size.

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can be added but can not be edited or deleted.



56. Storage and Handling Type

FDA GUDID

Description	Indicates storage and handling requirements that are required for the device including temperature, humidity, and atmospheric pressure. <b>SPL Definition: "Indicates storage requirements are required for the device, including: temperature, humidity, etc."</b>
Data Entry Notes	<b>Choose a value from the drop down LOV.</b> <b>Conditions of the Storage and Handling Type are measured below as a range, with a Low Value and a High Value. More than one Storage and Handling Type can be added per device record.</b>
Edit Rules After Grace Period	<b>Add (Addition of new data is allowed)</b> <b>Delete (Deletion of entered data is allowed)</b> <b>Edit (Editing of entered data is allowed)</b>
Required?	<b>Optional, SPL Text: "1..1"</b>
Data Type & Length	<b>NA</b>
Entry List of Values (LOV) –	<b>CV for Storage Conditions – Storage environment temperature; Storage environment humidity; Storage environment atmospheric pressure; Handling environment temperature; Handling environment humidity; Handling environment atmospheric pressure</b>
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Attribute Name- LOGICAL POPULATION- (Logical value based on the attribute (single or pair) chosen to be populated for the device.)

The list of applicable attributes are:

Current Attributes

Attribute Name-

- a. storageHandlingTemperatureMaximum
- b. storageHandlingTemperatureMinimum
- c. storageHandlingHumidityMaximum
- d. storageHandlingHumidityMinimum
- e. transportationMaximumTemperature
- f. transportationMinimumTemperature

Definition

- a. The maximum temperature at which the trade item can be stored. This uses a measurement consisting of a unit of measure and a value.
- b. The minimum temperature at which the trade item can be stored. This uses a measurement consisting of a unit of measure and a value.
- c. The maximum humidity in percentages that the goods should be stored in.



Storage environment atmospheric pressure	storageEnvironmentAtmosphericPressureMaximum; storageEnvironmentAtmosphericPressureMinimum	AVP
Handling environment temperature	transportationMaximumTemperature; transportationMinimumTemperature	
Handling environment humidity	transportationMaximumHumidityMaximum; transportationMaximumHumidityMinimum	AVP
Handling environment atmospheric pressure	transportationEnvironmentAtmosphericPressMaximum; transportationEnvironmentAtmosphericPressMinimum	AVP

Some devices have a temperature, humidity, or pressure range (High/Max and Low/Min values). Some have a greater than or less than value and others have a single or recommended value. Population of all possibilities can be handled in the GDSN and the GUDID using the following chart:

Information Type Available	Populated In	Value
Range of Lowest to Highest	Minimum or Low Values Field	Lowest Value
	Maximum or High Values Field	Highest Value
Less Than a Value	Minimum or Low Values Field	Leave Null (provide no value)
	Maximum or High Values Field	Highest Value
Greater Than a Value	Minimum or Low Values Field	Lowest Value
	Maximum or High Values Field	Leave Null (provide no value)
Single or Recommended Value	Minimum or Low Values Field	Single/Same Value populated in both fields
	Maximum or High Values Field	

57. Low Value **SPL Name: "Storage and Handling Low Value"**

FDA GUDID

Description	Indicates the low value for storage and handling requirements. <b>SPL Definition: "Indicates the low value for storage requirements, such as temperature, humidity, etc"</b>
Data Entry Notes	<b>Enter a number for Low Value.</b> <b>Must enter at least one value, Low or High but can enter both Low Value and High Value, if needed.</b>
Edit Rules After Grace Period	<b>Add (Addition of new data is allowed)</b> <b>Delete (Deletion of entered data is allowed)</b> <b>Edit (Editing of entered data is allowed)</b>
Required?	<b>Conditionally Required* *One value (Low or High) is required if Storage and Handling Type is added to the device record.</b>
Data Type & Length	<b>Type: Num.</b> <b>Length: 6</b>
Entry List of Values (LOV)	<b>NA</b>
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Attribute Name LOGICAL POPULATION- (Logical value based on the attribute (single or pair) chosen to be populated for the device.)

The list of applicable attributes are:

Current Attributes

Attribute Name

- a. storageHandlingTemperatureMinimum
- b. storageHandlingHumidityMinimum
- c. transportationMinimumTemperature

Definition

- a. The minimum temperature at which the trade item can be stored. This uses a measurement consisting of a unit of measure and a value.
- b. The minimum humidity in percentages that the goods should be stored in.
- c. The minimum temperature that a trade item can be held below during transport as defined by the manufacturer without affecting product safety or quality.

Temporary Attributes

Attribute Name

- a. storageEnvironmentAtmosphericPressureMinimum
- b. transportationEnvironmentAtmosphericPressMinimum
- c. transportationMaximumHumidityMinimum

**Definition**

- a. The minimum atmospheric pressure in which the item should be stored to remain usable. This value is the value below which the trade item should not be subjected.
- b. The minimum atmospheric pressure in which the item should be transported to remain usable. This value is the value below which the trade item should not be subjected.
- c. The minimum humidity in percentages in which the trade items should be transported.

Data Type	Measurement
GDSN Required	OPTIONAL

**Population Guidance (below)**

The GDSN attributes are pairs of attributes with a minimum and a maximum value. This provides a range of applicability for the device for that temperature/humidity/pressure pair. The applicable storage type can be derived from the attribute name.

For the GUDID, the GDSN attributes with “maximum” in their name will map the numeric value into the GUDID attribute High Value. The GDSN attributes with “minimum” in their name will map the numeric value into the GUDID attribute Low Value.

The following grid maps the GUDID code value for Storage Type to the applicable GDSN Attributes:

GUDID Storage Type Code	GDSN Attributes	
Storage environment temperature	storageHandlingTemperatureMaximum; storageHandlingTemperatureMinimum	
Storage environment humidity	storageHandlingHumidityMaximum; storageHandlingHumidityMinimum	
Storage environment atmospheric pressure	storageEnvironmentAtmosphericPressureMaximum; storageEnvironmentAtmosphericPressureMinimum	AVP
Handling environment temperature	transportationMaximumTemperature; transportationMinimumTemperature	
Handling environment humidity	transportationMaximumHumidityMaximum; transportationMaximumHumidityMinimum	AVP
Handling environment atmospheric pressure	transportationEnvironmentAtmosphericPressMaximum; transportationEnvironmentAtmosphericPressMinimum	AVP

Some devices have a temperature, humidity, or pressure range (High/Max and Low/Min values). Some have a greater than or less than value and others have a single or recommended value. Population of all possibilities can be handled in the GDSN and the GUDID using the following chart.

Information Type Available	Populated In	Value
Range of Lowest to Highest	Minimum or Low Values Field	Lowest Value
	Maximum or High Values Field	Highest Value
Less Than a Value	Minimum or Low Values Field	Leave Null (provide no value)
	Maximum or High Values Field	Highest Value

Information Type Available	Populated In	Value
Greater Than a Value	Minimum or Low Values Field	Lowest Value
	Maximum or High Values Field	Leave Null (provide no value)
Single or Recommended Value	Minimum or Low Values Field	Single/Same Value populated in both fields
	Maximum or High Values Field	

58. High Value **SPL Name: "Storage and Handling High Value"**

FDA GUDID

Description	Indicates storage and handling requirements that are required for the device including temperature, humidity, and atmospheric pressure. <b>SPL Definition: "Indicates the high value for storage requirements, such as temperature, humidity, etc"</b>
Data Entry Notes	<b>Enter a number for High Value.</b> <b>Must enter at least one value, Low or High but can enter both Low Value and High Value, if needed.</b>
Edit Rules After Grace Period	<b>Add (Addition of new data is allowed)</b> <b>Delete (Deletion of entered data is allowed)</b> <b>Edit (Editing of entered data is allowed)</b>
Required?	<b>Conditionally Required* *One value (Low or High) is required if Storage and Handling Type is added to the device record.</b>
Data Type & Length	<b>Type: Num.</b> <b>Length: 6</b>
Entry List of Values (LOV) –	<b>NA <del>CV for Storage Conditions– Storage environment temperature; Storage environment humidity; Storage environment atmospheric pressure; Handling environment temperature; Handling environment humidity; Handling environment atmospheric pressure</del></b>
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Attribute Name- LOGICAL POPULATION- (Logical value based on the attribute (single or pair) chosen to be populated for the device.) The list of applicable attributes are:

Current Attributes

Attribute Name-

- a. storageHandlingTemperatureMaximum
- b. storageHandlingHumidityMaximum
- c. transportationMaximumTemperature

Definition

- a. The maximum temperature at which the trade item can be stored. This uses a measurement consisting of a unit of measure and a value.
- b. The maximum humidity in percentages that the goods should be stored in.
- c. The maximum temperature that a trade item can be held at during transport as defined by the manufacturer without affecting product safety or quality.

Temporary Attributes

Attribute Name

- a. storageEnvironmentAtmosphericPressureMaximum





Information Type Available	Populated In	Value
Less Than a Value	Minimum or Low Values Field	Leave Null (provide no value)
	Maximum or High Values Field	Highest Value
Greater Than a Value	Minimum or Low Values Field	Lowest Value
	Maximum or High Values Field	Leave Null (provide no value)
Single or Recommended Value	Minimum or Low Values Field	Single/Same Value populated in both fields
	Maximum or High Values Field	

59. Unit of Measure SPL Name: "Storage and Handling Unit of Measure"

FDA GUDID

Description	The unit of measure associated with the storage and handling conditions.
Data Entry Notes	Choose a value from the drop down <b>LOV</b> . (Webtool)
Edit Rules After Grace Period	<b>Add (Addition of new data is allowed)</b> <b>Delete (Deletion of entered data is allowed)</b> <b>Edit (Editing of entered data is allowed)</b>
Required?	Conditionally Required* *Required if Storage and Handling Type is added to the device record
Data Type & Length	NA
Entry List of Values (LOV)	
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Attribute Name	N/A- UoMs for these values are built into the GDSN Attributes as they are of a data type of Measurement. A Measurement field has a numeric value and a qualifier (UoM)
----------------	--

Definition-

Data Type

GDSN Required

Population Guidance (below)

Potential UoMs for these storage and handling values are listed in Section 5 FDA GUDID mapping to GS1 code values under the UoM portion.

60. Special Storage Conditions

FDA GUDID

Description	Indicates any special storage requirements for the product. <b>SPL Text: "Indicates any special storage requirements for the product."</b>
Data Entry Notes	<b>Enter any other storage conditions.</b> <b>For devices kept at room temperature, or other standard conditions, input that information here.</b>
Edit Rules After Grace Period	<b>Add (Addition of new data is allowed)</b> <b>Delete (Deletion of entered data is allowed)</b> <b>Edit (Editing of entered data is allowed)</b>
Required?	<b>Conditionally Required*</b> <b>*Required if 'Special Storage Conditions' is selected above</b>
Data Type & Length	<b>Type: Alphanum.</b> <b>Length: 200</b>
Entry List of Values (LOV)	<b>NA</b>
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Attribute Name	consumerUsageStorageInstructions
Definition-	Expresses in text the consumer storage and usage instructions of a product which are normally held on the label or accompanying the product. This information may or may not be labelled on the pack. Instructions may refer to a suggested storage temperature, a specific storage requirement or a reference to environment or duration. Examples include: "Refrigerate After Opening", "Consume within 4 days" "Keep Out Of Direct Sunlight", "Store at an Ambient Temperature", "Store in a Clean, Cool, Dry Place", "Store Away From Sunlight, Strong Odours and Chemicals", "Keep in a Clean, Cool, Dry and Odourless Place Away From Direct Sunlight and Freezing Temperatures", "Keep in a Clean, Cool, Dry and Odourless Place Away From Direct Sunlight", "Before opening store at + 5°C+ 30°C", "After Opening Keep Refrigerated (+5°C) and Consume Within 48 hours", "Drink Chilled", "Store in a Cool Dry Place", "Refrigerate After Opening. Can Be Kept in the Fridge For 3 Months".
Data Type	Text (Language qualified) (1-1000 characters)
GDSN Required	OPTIONAL

Population Guidance (below)

This attribute can be populated with any special storage, transportation, or handling instructions as deemed necessary by the supplier/manufacturer.

61. Device Packaged as Sterile

FDA GUDID

Description Indicates the medical device is free from viable microorganisms. See ISO/TS 11139.

Data Entry Notes **Choose Yes/No from the drop down list.**

**The two Sterilization Method questions are independent of each other; this element is designed to capture information about the device as it enters Commercial Distribution. These data elements are not designed to capture sterilization procedures executed by the manufacturer or labeler.**

Edit Rules After Grace Period **None (NO edit, add, or delete are allowed)**

Required? **Required**

Data Type & Length **Type: Boolean**

Entry List of Values (LOV) Yes/No

New DI Trigger? YES

Public/Private Status Public

GS1 GDSN

Attribute Name initialManufacturerSterilisation

LOGICAL POPULATION (Logical BOOLEAN value of TRUE from the population of any value in initialManufacturerSterilisation)

Definition- Type(s) of sterilisation that may have been performed by the manufacturer if a trade item is sterile when it comes from the manufacturer. Sterilisation refers to any process that effectively kills or eliminates transmissible agents (such as fungi; bacteria; viruses; prions and spore forms etc.) from a surface; equipment; foods; medications; or biological culture medium. Some methods of sterilisation are through the application of heat; radiation; and ethylene.

Data Type Code List

GDSN Required OPTIONAL

Population Guidance (below)

This GDSN attribute is a code list. If a value is published in GDSN, it indicates that the device is sold as being sterile. Therefore if a value is published in the GDSN attribute initialManufacturerSterilization, then a value of "TRUE" will be populated in the GUDID. If no value is published in GDSN, then a value of "FALSE" will be populated in the GUDID.

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can not be changed. Many of the data elements are locked and can no longer be edited.

62. Requires Sterilization Prior to Use

FDA GUDID

Description	Indicates that the device requires sterilization prior to use.
Data Entry Notes	<p>Choose Yes/No from the drop down list.</p> <p>The two Sterilization Method questions are independent of each other; this element is designed to capture information about the device before it can safely encounter a patient, regardless of whether the device is single use or reused after reprocessing. These data elements are not designed to capture sterilization procedures executed by the manufacturer or labeler.</p> <p>If answered 'Yes', at least one Sterilization Method (below) must be selected.</p>
Edit Rules After Grace Period	None (NO edit, add, or delete are allowed)
Required?	Required
Data Type & Length	Type: Boolean
Entry List of Values (LOV)	Yes/No
New DI Trigger?	NO
Public/Private Status	Public

GS1 GDSN

Attribute Name	LOGICAL POPULATION- (Logical BOOLEAN value of TRUE from the population of any value in initialSterilisationPriorToUse)
Definition	N/A
Data Type	N/A
GDSN Required	OPTIONAL

Population Guidance (below)

The GDSN attribute initialSterilizationPriorToUse is a code list indicating the type(s) of sterilization which should be performed on a device prior to use. Population of a value for this attribute signifies that the device is not sterile and that the Provider does need to sterilize it prior to use using the method populated. If a code value is published in the GDSN, then a value of "TRUE" will be populated in the GUDID. If no value is published in GDSN, then a value of "FALSE" will be populated in the GUDID.

Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can not be changed. Many of the data elements are locked and can no longer be edited.

63. Sterilization Method

FDA GUDID

Description Indicates the method(s) of sterilization that can be used for this device.

Data Entry Notes **Choose a value from the drop down LOV.**

**Only applicable if the answer to 'Requires Sterilization Prior to Use' is 'Yes'; otherwise, the LOV will remain inactive.**

**The Entry LOVs represent the sterilization methods recognized by the CDRH Infection Control Branch. Methods selected should be only those approved for each device by the CDRH Office of Device Evaluation.**

Edit Rules After Grace Period **Add (Addition of new data is allowed)**

**Delete (Deletion of entered data is allowed)**

**Edit (Editing of entered data is allowed)**

Required? **Conditionally Required\***

**\*if 'Requires Sterilization Prior to Use' is marked 'Yes'**

Data Type & Length **NA**

Entry List of Values (LOV) – **Chlorine Dioxide; Dry Heat; Ethylene Oxide; High Intensity Light or Pulse Light; Hydrogen Peroxide; Microwave Radiation; Moist Heat or Steam; Ozone; Peracetic Acid; Radiation; Sound Waves; Ultraviolet Light**

New DI Trigger? **NO**

Public/Private Status **Public**

GS1 GDSN

Attribute Name **initialSterilisationPriorToUse**

Definition- **This is an indication of the type(s) of sterilisation that is required to be completed by a healthcare provider prior to initial use of the healthcare trade item. Sterilisation refers to any process that effectively kills or eliminates transmissible agents (such as fungi; bacteria; viruses; prions and spore forms etc.) from a surface; equipment; foods; medications; or biological culture medium. Some methods of sterilisation are through the application of heat; radiation; and ethylene.**

Data Type **Code List**

GDSN Required **OPTIONAL**

Population Guidance (below)

**This GDSN attribute is a code list of the type(s) of sterilization, which can be performed on a device by the Provider prior to use. When this attribute is published, a value of "TRUE" will be populated for the GUDID attribute Requires Sterilization Prior to Use. It is recommended to not use the value of UNSPECIFIED as the FDA GUDID will not accept that value.**



Once published, a 7-day grace period begins. During the grace period, most attributes can be edited. After the grace period ends on day 8, this attribute can be edited, but only under certain circumstances. See [Edit Rules After Grace Period](#) for more details

## 7. References

- For more information on UDI at a global level refer to <http://www.gs1.org/healthcare/udi>
- For more information on the IMDRF refer to <http://www.imdrf.org/>
- For more information on the U.S. FDA UDI refer to <http://www.gs1us.org/industries/healthcare/gs1-healthcare-us/fda-udi>
- For more information on the GDSN refer to <http://www.gs1.org/gdsn>
- For more information on GS1 Healthcare refer to <http://www.gs1.org/healthcare>
- For country support contact your local GS1 Member Organisation <http://www.gs1.org/contact>
- For an interactive spreadsheet of the mapping from GDSN to FDA GUDID refer to [http://www.gs1us.org/gs1-us-library?Command=Core\\_Download&EntryId=747](http://www.gs1us.org/gs1-us-library?Command=Core_Download&EntryId=747)